



505 - 6th Street, Suite 200  
New Westminster, BC V3L 0E1

Toll Free: 1-866-566-SAFE  
Fax: (778) 396 - 2064  
www.safetyauthority.ca

PRESSURE VESSEL ENGINEERING  
B-120 RANDALL DRIVE  
WATERLOO ON N2V 1C6

**Date:** October 17, 2014  
**Account #:** 45363  
**Journal #:** 60627  
**Our File #:** 5511261

**Attn:** CATHERINE DIPLOCK

**Re:** Application for Design Registration

The design, as detailed in your, PVE-8217, for a Fitting is accepted for registration as follows:

**Registered To:** KURZ INSTRUMENTS INC **CRN:** 0F06882.21

**Drawing #:** Series 454FTB

**Drawing Revision:**

**Conditions Of Registration:**

Registration of Series 454FTB Insertion Mass Flow Transmitters.

This design was registered based on a technical review performed by the province of initial registration in accordance with the Association of Chief Inspectors policy on reciprocal recognition of design review.

**Reviewer's Notes:**

As required by CSA B51 4.2.1, this registration expires on August 28, 2024. This CRN is valid until the expiry date as long as the Manufacturer maintains a valid quality control program verified by an acceptable third-party agency until that date. Should the certification of the quality control program lapse before the expiry date, this registration shall become void.

Contact me if you have any questions. The invoice for registration will be forwarded under separate cover.

SHARON PETERS

boiler.designregistration@safetyauthority.ca  
Design Administration

**cc:**

<b>Pressure Vessel Engineering Ltd.</b> info@pveng.com www.pveng.com	<b>Document Transmittal</b>	120 Randall Drive, Suite B Waterloo, Ontario Canada N2V 1C6
--	-----------------------------	--

**Attention: Daniel Kurz**

To:	Kurz Instruments Inc.
Address:	2411 Garden Road Monterey CA USA 93940
Date:	04/08/15
Phone:	831-646-5911 x314
Fax:	831-646-8901

From:	Pressure Vessel Engineering
Job / Ref:	PVE-8217 Series 454FTB Insertion Mass Flow Transmitters
Admin Contact:	Catherine Diplock, cmd@pveng.com
Phone:	(519) 880-9808 ext 226
Fax:	(519) 880-9810
Technical Contact:	Kevin Myers, kcm@pveng.com
Phone:	(519) 880-9808 ext 246
Fax:	(519) 880-9810
Via:	UPS

Please find enclosed the following documents

Item #	Description	Comment / Status	Qty
1			
2			
3			
4			
5	Canada Wide CRN documents		1
6			
7			
8			
9			
10			
11			
12			

Dear Daniel Kurz,

Please find all listed items enclosed in this package. If there are any issues please contact Pressure Vessel Engineering using the above contact information.

Regards,

Catherine Diplock



the pressure equipment safety authority

9410 - 20 Ave N.W.  
Edmonton, Alberta, Canada T6N 0A4  
Tel: (780) 437-9100 / Fax: (780) 437-7787

August 28, 2014

**Attention:** Catherine Diplock  
PRESSURE VESSEL ENGINEERING INC  
120 RANDALL DRIVE SUITE B  
WATERLOO, ON N2V 1C6

The design submission, tracking number 2014-05500, originally received on July 09, 2014 was surveyed and accepted for registration as follows:

**CRN :** 0F06882.2

**Accepted on:** August 28, 2014

**Reg Type:** Addition to Acc. Fitting

**Expiry Date:** August 28, 2024

**Drawing No. :** PVESCP-8217-1.0

**Fitting type:** SERIES 454FTB MASS FLOW TRANSMITTERS

Design registered in the name of : KURZ INSTRUMENTS

**The registration is conditional on your compliance with the following notes:**

*The CRN renewal is given based on the understanding that there is no change to the originally registered design.*

*This registration is valid only for fittings fabricated at the location(s) covered by the QC certificate attached to the accepted AB-41 Statutory Declaration form. This registration is valid only until the indicated expiry date only if the Manufacturer maintains a valid quality management system approved by an acceptable third-party agency until that date. Should the approval of the quality management system lapse before the expiry date indicated above, this registration shall become void.*

An invoice covering survey and registration fees will be forwarded from our Revenue Accounts.

Enclosed are stamped prints for your reference.

Sincerely,

ONSHCHENKO, TETYANA, P. Eng.



**ABSA**  
the pressure equipment safety authority  
**STATUTORY DECLARATION**  
**Registration of Fittings**

In this space, show facsimile of manufacturer's logo or trademark as it will appear on the fitting.




I, Daniel Kurz,

General Manager

(company title, e.g. vice president, plant manager, chief engineer) (must be in a position of authority)

of Kurz Instruments  
(name of manufacturer)

located at 2411 Garden Road, Monterey, CA, 93940, USA  
(plant address)

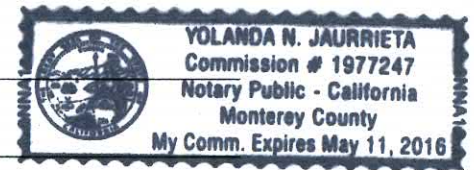

do solemnly declare that the fittings listed hereunder, which are subject to the Safety Codes Act (check one)

- ☐ comply with the requirements of \_\_\_\_\_ which specifies the dimensions,  
(title of recognized North American Standard)  
materials of construction, pressure/temperature ratings and identification marking of the fittings, or
- ☒ are not covered by the provisions of a recognized North American standard and are therefore manufactured to comply with ASME B31.3 2012 EDITION as supported by the attached data which identifies the dimensions, materials of construction, pressure/temperature ratings and the basis for such ratings, and the marking of the fittings for identification.

I further declare that the manufacture of these fittings is controlled by a quality control program which has been verified by the following authority, FM Approvals as being suitable for the manufacture of these fittings to the stated standard. The fittings covered by this declaration, for which I seek registration, are Series 454FTB Insertion Mass Flow Transmitters

In support of this application, the following information, calculations and/or test data are attached:

PVEscp-8217-1

DECLARED before me at California in the County of Monterey  
this 25 day of June, 2014  
(Month) (Year)  
(print) Yolanda N. Jaurrieta  
(sign) Yolanda N. Jaurrieta  
(A Commissioner for Oaths)

**See Acceptance Letter for the comments and/or conditions of registration.**

**For Office Use Only**

To the best of my knowledge and belief, the application meets the requirements of the Safety Codes Act and CSA Standard B51, Clause 4.2, and is accepted for registration in Category F

Registration Number: 06882.2

Date Registered: AUG 28 2014

(For the Administrator/Chief Inspector of Alberta)

Expiry Date: August 28, 2024

The information you provide is necessary only for the administration of the programs as required by the Alberta Safety Codes Act and Regulations in the Boiler Discipline.





**Inspection and Technical Services Manitoba**  
500 - 401 York Avenue  
Winnipeg Manitoba R3C 0P8  
T (204) 945-3373  
F (204) 948-2309  
[www.firecomm.gov.mb.ca/codes\\_steam\\_pressure.html](http://www.firecomm.gov.mb.ca/codes_steam_pressure.html)

13 November, 2014

Pressure Vessel Engineering  
Suite B-120 Randall Drive  
Waterloo, ON  
N2V 1C6

Attn: Catherine Diplock

### **REGISTRATION OF VALVES AND FITTINGS**

**Manufacturer:** Kurz Instruments Inc.

The design(s) for the following Valves/Fittings has been received by us and has been examined and accepted for registration in the Province of Manitoba as follows.

<b>DRAWING / CATALOGUE</b>	<b>CRN</b>	<b>FILE</b>
PVEscp-8217-1.0	0F06882.24	34540

**An invoice covering survey and registration fees is enclosed.**

***NOTE:** CRN registered under reciprocal agreement & is conditional based on compliance with the notes set by the original issuing Jurisdiction: **ABSA**. See attached stamped "this is part of CRN" for scope of registration. This registration expires **August 28, 2024**.*

This registration is valid until the indicated expiry date only if the Manufacturer maintains a valid quality management system approved by an acceptable third-party agency until that date. Should the approval of the quality management system lapse before the expiry date indicated above, this registration shall become void.

The registration of this design does not relieve the manufacturer, the owner or his agent of the responsibility for the design or construction of a fitting in accordance with the applicable Acts, Codes and Standards. Inspection and Technical Services assumes no responsibility by registering designs, examining plans and/or inspecting equipment or facility.

Yours truly,

**Rabie Harb, E.I.T.**  
Design Surveyor  
Office of the Fire Commissioner  
Inspection and Technical Services Manitoba  
500 - 401 York Avenue  
Winnipeg, Manitoba, R3C 0P8  
Phone: 204-945-3373  
Email: [rabie.harb@gov.mb.ca](mailto:rabie.harb@gov.mb.ca)

# MANITOBA

DEPARTMENT OF LABOUR  
AND IMMIGRATION  
500 - 401 York Avenue  
Winnipeg, Manitoba R3C 0P8



## STATUTORY DECLARATION REGISTRATION OF FITTINGS

### (a) Design Qualification

I, Daniel Kurz  
(See Note 2)

General Manager

(Position e.g.: president, plant manager, chief eng.)

of Kurz Instruments

(Name of company)

located at 2411 Garden Road, Monterey, CA, 93940, USA

(Plant Address)

do solemnly declare that the fittings listed hereunder, which are subject to the Boilers & Pressure Vessels Act,

comply with all the requirements of the ANSI/ASME codes as to their dimensions.

or

- ☒ are not covered by the provisions of the ANSI/ASME codes, and are therefore constructed to comply with  
ASME B31.3 2012 EDITION code or standard, and are designed to the best current  
engineering practice, as shown by the supporting test data.

### (b) Quality Control of Manufacture

I further declare the manufacture of these fittings is controlled by a quality control program which complies with the requirements of  
ISO, and has been verified by the following authority or authorized agency FM Approvals  
9001:2008

The fittings covered by this declaration, for which I seek registration, are Series 454FTB Insertion Mass Flow Transmitters

In support of the application, the following information, calculations and/or test data are attached:

PVEscp-8217-1

Declared before me at California in the province/state of County of Monterey the 25  
day of June AD 20 14

A (commissioner for oaths)

Yolanda N. Jaurrieta

Signature of Declarer

### (For Official Use Only)

The application is accepted for registration in Category "F" in accordance with the Boilers and Pressure Vessels Act  
and CSA Standard B51.

This registration must be revalidated after ten (10) years from the date of acceptance.

August 28, 2024

Registered Number CRN ØFØ6882.21

For the Chief Inspector

Ralph Hall

Date:

Nov 13, 2014



YOLANDA N. JAURRIETA  
Commission # 1977247  
Notary Public - California  
Monterey County  
My Comm. Expires May 11, 2016

### Notes:

- (1) This form shall be completed and signed by the president or highest official in the manufacturing plant where the fitting is produced.
- (2) Two completed copies of Statutory Declaration form together with two copies of Catalogs, drawings or Bulletins illustrating above fittings shall be submitted.
- (3) All fittings are required to be registered in the name of the Manufacturer.



14th Floor, Centre Tower  
3300 Bloor Street West  
Toronto, Ontario  
Canada M8X 2X4  
Tel.: 416.734.3300  
Fax: 416.231.1626  
Toll Free: 1.877.682.8772

[www.tssa.org](http://www.tssa.org)

October 08, 2014

CATHERINE DIPLOCK  
PRESSURE VESSEL ENGINEERING LTD.  
120 RANDALL DR SUITE B  
WATERLOO ON N2V 1C6  
CA

**Service Request Type:** BPV-Fitting Registration  
**Service Request No.:** 1484224  
**Your Reference No.:** PVE-8217  
**Registered to:** KURZ INSTRUMENTS INC

Dear CATHERINE DIPLOCK,

Technical Standards and Safety Authority (TSSA) is pleased to inform you that your submission has been reviewed and registered as follows:

**CRN No.:** 0F06882.25R1

Main Design No.: CRN Renewal for SERIES 454FTB INSERTION MASS FLOW TRANSMITTERS  
Expiry Date: 28-Aug-2024

Please be advised that a valid quality control system must be maintained for the fitting registration to remain valid until the expiry date.

**NOTE: There is no change in the original design of the subject valve series.**

The stamped copy of the approved registration and the invoice are mailed separately. Should you have any questions or require further assistance, please contact a Customer Service Advisor at 1.877.682.TSSA (8772) or e-mail [customerservices@tssa.org](mailto:customerservices@tssa.org). We will be happy to assist you. When contacting TSSA regarding this file, please refer to the Service Request number provided above.

Yours truly,

Mark Valcic P. Eng.  
Engineer BPV  
Tel.: 416-734-3494  
Fax: 416-231-6183  
Email: [mvalcic@tssa.org](mailto:mvalcic@tssa.org)





TECHNICAL STANDARDS &  
SAFETY AUTHORITY  
14th Floor, Centre Tower  
3300 Bloor Street West  
Toronto, Ontario  
Canada M8X 2X4

Show facsimile of manufacturer's logo or trademark, as it will  
appear on the fitting, in the space below



## STATUTORY DECLARATION

### Registration of Fittings

I, Daniel Kurz General Manager

(Name and Position, e.g. President, Plant Manager, Chief Engineer)

of Kurz Instruments

(Name of Manufacturer)

Located at 2411 Garden Road, Monterey, CA, 93940, USA

(Plant Address)

(831)-646-5911

(Telephone No.)

(831)-646-8901

(Fax No.)

☐ do solemnly declare that the fittings listed hereunder, which are subject to the **Technical Standards and Safety Act**, Boilers and Pressure Vessels Regulation, comply with all of the requirements of

(Title of recognized North American Standard)

which specifies the dimensions, materials of construction, pressure/temperature ratings, identification marking the fittings and service;

☒ or are not covered by the provisions of a recognized North American standard and are therefore manufactured to comply with ASME B31.3 2012 EDITION as supported by the attached data which identifies the dimensions, material of construction, pressure/temperature ratings and the basis for such ratings, the marking of the fitting for identification and service.

I further declare that the manufacture of these fittings is controlled by a quality system meeting the requirements of ISO 9001:2008 which has been verified by the following authority, FM Approvals.

The items covered by this declaration, for which I seek registration, are category F type fittings. In support of this application, the following information and/or test data are attached as follows:

PVEscp-8217-1

(drawings, calculations, test reports, etc.)

Declared before me at Monterey County in the State of California

the 25 day of June AD 20 14.


Commissioner for Oaths:

Yolanda N. Jaurrieta

(Printed name)

Yolanda N. Jaurrieta

(Signature)

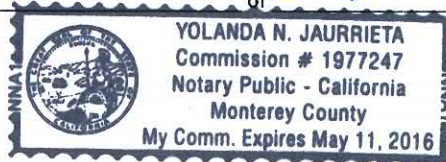

[Signature]

(Signature of Declarant)

#### FOR OFFICE USE ONLY

To the best of my knowledge and belief, the application meets the requirements of the **Technical Standards and Safety Act**, Boilers and Pressure Vessels Regulation, and CSA Standard B51 and is accepted for registration in Category F1.

CRN:

OF06882.25R1

Registered by:

MARK VALCIC, P.Eng.

Dated:

OCT. 8, 2014

NOTE: This registration expires on

AUG 28, 2024

PV 0953 (0504)

NOTE: SERIES 459 FTB Insertion MASS FLOW TRANSMITTERS

Technical  
Standards  
and Safety  
Authority

Boilers and  
Pressure Vessels  
Safety Program

REGISTERED

C.R.N.:

OF06882.25R1

Signed:

[Signature]

Date:

OCT. 8, 2014

OCT 8/14

Le 26 mars 2015.

MR. KEVIN MYERS  
PRESSURE VESSEL ENGINEERING LTD  
120 RANDAL DR., SUITE B  
WATERLOO ONTARIO  
CANADA N2V 1C6

REFERENCE : C.R.N. application  
CATALOGUE SERIES 454 FTB  
PVESCP-8217-1.0

SERIES 454 FTB MASS FLOW TRANSMITTERS 1/2" TO 4"

OUR REFERENCE : 958466

MANUFACTURER : KURZ INSTRUMENTS, INC.  
2411 GARDEN ROAD  
MONTEREY CALIFORNIA  
U.S.A. 93940

Dear Sir,

According to our law respecting pressure vessels, your plans have been accepted and registered under the number 0F06882.26.

*TS for*

GILLES BONNIER

Inspecteur

Service de l'inspection de la fabrication  
d'appareils sous pression  
545, boulevard Crémazie est, 7<sup>ème</sup> étage  
Montréal (Québec) Canada  
H2M 2V2

Téléphone : (514) 873-6459  
Sans frais : 1 866 262-2084  
Télécopieur : (514) 873-9936

# Statutory Declaration Registration of Fittings



## (a) Design Qualification

I<sup>1</sup> Daniel Kurz  
General Manager  
(Position eg. president, plant manager, chief eng.)

Of Kurz Instruments  
(name of company)

Located at 2411 Garden Road, Monterey, CA, 93940, USA  
(plant address)

do solemnly declare that the fittings listed hereunder, which are subject to the Boilers & Pressure Vessels Act:

☐ comply with all the requirements of the ANSI/ASME codes as to their dimensions, material, identification & service for which are required:

Or

☒ are not covered by the provisions of the ANSI/ASME codes, and are therefore constructed to comply with ASME B31.3 2012 EDITION  
code and standard, and are designed to the best current engineering practice, as shown by the supporting test data.

## (b) Quality control of Manufacture

I further declare the manufacture of these fittings is controlled by a quality control program which complies with the requirements of ISO 9001:2008, and has been verified by the following authority or authorized agency FM Approvals

The fittings<sup>2</sup> covered by this declaration, for which I seek registration, are Series 454FTB Insertion Mass Flow Transmitters

In support of the application, the following information, calculations and/or test data are attached:  
PVEscp-8217-1


Declared before me at California

In the of County of Monterey

The 25 Day of June AD 19 2014

Yolanda N. Jaurrieta  
A (commissioner for paths)

[Signature]  
Signature of Declarer<sup>3</sup>

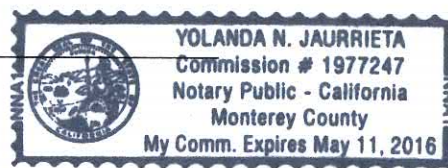

For Official Use Only	
The application is accepted for registration in Category <u>F</u> in accordance with the Boilers and Pressure Vessels Act and CSA Standard B51.	
This registration must be revalidated after ten (10) years from the date of acceptance.	
Registered Number CRN <u>06882.26</u>	For the Chief Inspector <u>[Signature]</u>
	Date <u>28 NOV. 2014</u>

- Three completed copies of Statutory Declaration form together with three copies of Catalogs, drawings of Bulletins illustrating above fittings shall be submitted.
- All fittings are required to be registered in the name of the Manufacturer.
- This form shall be completed and signed by the president or highest official in the manufacturing plant where the fitting is produced.



**REVISION**  
**OF 06882.26**

28 NOV. 2014

## Kurz Instruments - Series 454FTB Insertion Mass Flow Transmitters

**PVEscp-8217-1.0**

This submission is a re-registration of fittings using CSA B51-14 Part 1 4.2.8(c) method.

The current registration uses the exact pressure retaining components of the previous CRN registration 0F06882.2

Model Number

454FTB-08-MT	Flange Size	316 SS SA-240 316L Plate	304 SS SA-240 304L Plate	Hastalloy C276 SB-575 Alloy N10276	Monel SB-127 Alloy N04400
	1/2" Class 150	YES	YES	YES	YES
	1/2" Class 300	YES	YES	YES	YES
	3/4" Class 150	YES	YES	YES	YES
	3/4" Class 300	YES	YES	YES	YES
	1" Class 150	YES	YES	YES	YES
	1" Class 300	YES	YES	YES	YES
	1-1/2" Class 150	YES	YES	YES	YES
	1-1/2" Class 300	YES	YES	YES	YES
	2" Class 150	YES	YES	YES	YES
	2" Class 300	YES	YES	YES	YES
	3" Class 150	YES	YES	YES	YES
	3" Class 300	YES	YES	YES	YES
	4" Class 150	YES	YES	YES	YES
	4" Class 300	YES	YES	YES	YES

454FTB-08-HHT	Flange Size	316 SS SA-240 316L Plate	304 SS SA-240 304L Plate	Hastalloy C276 SB-575 Alloy N10276	Monel SB-127 Alloy N04400
	1/2" Class 150	NO	NO	YES	YES
	1/2" Class 300	NO	NO	YES	YES
	3/4" Class 150	NO	NO	YES	YES
	3/4" Class 300	NO	NO	YES	YES
	1" Class 150	NO	NO	YES	YES
	1" Class 300	NO	NO	YES	YES
	1-1/2" Class 150	NO	NO	YES	YES
	1-1/2" Class 300	NO	NO	YES	YES
	2" Class 150	NO	NO	YES	YES
	2" Class 300	NO	NO	YES	YES
	3" Class 150	NO	NO	YES	YES
	3" Class 300	NO	NO	YES	YES
	4" Class 150	NO	NO	YES	YES
	4" Class 300	NO	NO	YES	YES

454FTB-12-MT	Flange Size	316 SS SA-240 316L Plate	304 SS SA-240 304L Plate	Hastalloy C276 SB-575 Alloy N10276	Monel SB-127 Alloy N04400
	3/4" Class 150	YES	YES	YES	YES
	3/4" Class 300	YES	YES	YES	YES
	1" Class 150	YES	YES	YES	YES
	1" Class 300	YES	YES	YES	YES
	1-1/2" Class 150	YES	YES	YES	YES
	1-1/2" Class 300	YES	YES	YES	YES

454FTB-12-HHT	Flange Size	316 SS SA-240 316L Plate	304 SS SA-240 304L Plate	Hastalloy C276 SB-575 Alloy N10276	Monel SB-127 Alloy N04400
	3/4" Class 150	NO	NO	YES	YES
	3/4" Class 300	NO	NO	YES	YES
	1" Class 150	NO	NO	YES	YES
	1" Class 300	NO	NO	YES	YES
	1-1/2" Class 150	NO	NO	YES	YES
	1-1/2" Class 300	NO	NO	YES	YES

## UNIFORM STATUTORY DECLARATION FORM FOR THE REGISTRATION OF FITTING DESIGNS

NEW BRUNSWICK  
NUNAVUTNOVA SCOTIA  
YUKONPRINCE EDWARD ISLAND  
NORTHWEST TERRITORIES

NEWFOUNDLAND AND LABRADOR

MANUFACTURERS NAME: Kurz Instruments

MANUFACTURERS ADDRESS: 2411 Garden Road, Monterey, CA, 93940, USA

PLANT LOCATIONS:

CATEGORY OF FITTINGS TO BE REGISTERED. CIRCLE ONE CATEGORY ONLY

- A Pipe fittings, including couplings, tees, elbows, Ys, plugs, unions, pipe caps, or reducers  
 B Flanges: all flanges  
 C Valves: all line valves  
 D Expansion joints, flexible connections, and hose assemblies: all types  
 E Strainers, filters, separators, and steam traps  
 F Measuring devices, including pressure gauges, level gauges, sight glasses, levels, or pressure transmitters  
 G Certified capacity-rated pressure relief devices acceptable as primary over pressure protection on boilers, pressure vessels, piping and fusible plugs  
 H Pressure retaining components that do not fall into one of the above categories  
 N Nuclear components: Class 1 ☐ Class 2 ☐ Class 3 ☐ (Meeting CNSC or ASME requirements)

TITLE OF THE STANDARD OR SPECIFICATION

ASME B31.3 2012 EDITION

SHOW MANUFACTURERS NAME, TRADEMARK, OR LOGO AS IT WILL APPEAR ON THE PRODUCT



TYPE OF CONSTRUCTION

 FORGED ☐ WELDED ☒ WROUGHT ☐  
 CAST ☐ OTHER ☐  
 DESCRIBE OTHER:

LIST OF SUPPORTING DOCUMENTATION AND IDENTIFICATION OF THE ACTUAL ITEMS TO BE REGISTERED:

PVEscp-8217-1


Series 454FTD Insulation Mass Flow Transmitters

## DECLARATION:

I, Daniel Kurz, (hereinafter) employed by Kurz Instruments and being the person having full authority and responsibility for the quality of the and product do solemnly declare that the information contained in this form is true and to the best of my knowledge represents the product for which registration is sought. The dimensions, materials of construction, pressure temperature ratings, and identification markings are in accordance with the herein named standards. I further declare that the manufacture of these fittings is regulated by a Quality Control Program which extends to each plant where fabrication occurs in whole or in part and has been verified by FM Approvals as being suitable for that purpose and I make this solemn declaration conscientiously believing it to be true, and knowing that it is of the same force and effect as if made in open court.

Signature of Declarer: [Signature]Declared before me at Monterey County, CaliforniaThis 25 day of June AD 2014

Commissioner of Oaths

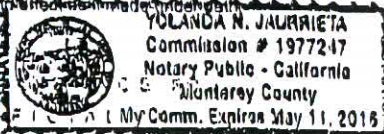or Notary Public (sign): [Signature]

This space for Regulatory Authority use

This registration must be revalidated after ten (10) years from the date of

CRN: OF06882.2 Add.1FID#: 2013

## Notes

1. All fittings shall be registered in the name of the Manufacturer.
2. Each category shall be supported with two Statutory Declaration forms and one copy of supporting documentation.
3. The declaration shall be made by the person having full authority and responsibility for the quality of the and product.
4. Quality control programs shall be resubmitted for validation at a maximum interval of five (5) years.


 ACCEPTED  
 PROVINCE OF PRINCE EDWARD ISLAND  
 ENVIRONMENT, LABOUR & JUSTICE
C.R.N. OF06882.29 Add 1DATE: Oct 3/14
 INSPECTION SERVICES SECTION  
 BOILER/PRESSURE VESSEL BRANCH



## UNIFORM STATUTORY DECLARATION FORM FOR THE REGISTRATION OF FITTING DESIGNS

NEW BRUNSWICK  
NUNAVUTNOVA SCOTIA  
YUKONPRINCE EDWARD ISLAND  
NORTHWEST TERRITORIES

NEWFOUNDLAND AND LABRADOR


MANUFACTURERS NAME: Kurz Instruments	
MANUFACTURERS ADDRESS: 2411 Garden Road, Monterey, CA, 93940, USA	
PLANT LOCATIONS:	
<b>CATEGORY OF FITTINGS TO BE REGISTERED. CIRCLE ONE CATEGORY ONLY</b> A Pipe fittings, including couplings, tees, elbows, Ys, plugs, unions, pipe caps, or reducers B Flanges: all flanges C Valves: all line valves D Expansion joints, flexible connections, and hose assemblies: all types E Strainers, filters, separators, and steam traps F Measuring devices, including pressure gauges, level gauges, sight glasses, levels, or pressure transmitters G Certified capacity-rated pressure relief devices acceptable as primary over pressure protection on boilers, pressure vessels, piping and fusible plugs H Pressure retaining components that do not fall into one of the above categories N Nuclear components: Class 1 <input type="checkbox"/> Class 2 <input type="checkbox"/> Class 3 <input type="checkbox"/> (Meeting CNSC or ASME requirements)	<b>TITLE OF THE STANDARD OF CONSTRUCTION</b> ASME B31.3 2012 EDITION
<b>SHOW MANUFACTURERS NAME, TRADEMARK, OR LOGO AS IT WILL APPEAR ON THE PRODUCT</b> 	
<b>TYPE OF CONSTRUCTION</b> FORGED <input type="checkbox"/> WELDED <input checked="" type="checkbox"/> WROUGHT <input type="checkbox"/> CAST <input type="checkbox"/> OTHER <input type="checkbox"/> DESCRIBE OTHER:	
<b>LIST OF SUPPORTING DOCUMENTATION AND IDENTIFICATION OF THE ACTUAL ITEMS TO BE REGISTERED:</b> PVEScp-B217-1 Series 454FIB Insertion Mass Flow Transmitters	

## DECLARATION:

I, Daniel Kurz, owner employed by Kurz Instruments and being the person having full authority and responsibility for the quality of the end product do solemnly declare that the information contained in this form is true and to the best of my knowledge represents the product for which registration is sought. The dimensions, materials of construction, pressure temperature ratings, and identification markings are in accordance with the herein named standards. I further declare that the manufacture of these fittings is regulated by a Quality Control Program which extends to each plant where fabrication occurs in whole or in part and has been verified by FM Approvals as being suitable for that purpose and I make this solemn declaration conscientiously believing it to be true, and knowing that it is of the same force and effect as if made under oath.

Signature of Declarer: [Signature]Declared before me at Monterey County in CaliforniaThis 25 day of June AD 2014

Commissioner of Oaths

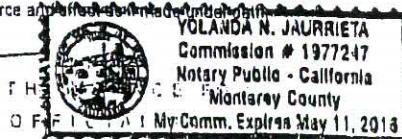or Notary Public (sign): [Signature]

This space for Regulatory Authority use This registration must be revalidated after ten (10) years from the date of acceptance.	
CRN: <u>OF06882.2 Add.1</u>	Date <u>Oct. 3/14</u> C.R.N. <u>OF06882.28ADD1</u> Dwg. <u>as described</u> Signed <u>[Signature]</u> 1 of 1 Part ACT & REGULATIONS
Notes: 1. All fittings shall be registered in the name of the Manufacturer. 2. Each category shall be supported with two Statutory Declaration forms and one copy of supporting documentation. 3. The declaration shall be made by the person having full authority and responsibility for the quality of the end product. 4. Quality control programs shall be resubmitted for validation at a maximum interval of five (5) years.	




# UNIFORM STATUTORY DECLARATION FORM FOR THE REGISTRATION OF FITTING DESIGNS

NEW BRUNSWICK  
NUNAVUT

NOVA SCOTIA  
YUKON

PRINCE EDWARD ISLAND  
NORTHWEST TERRITORIES

NEWFOUNDLAND AND LABRADOR

MANUFACTURERS NAME: Kurz Instruments	
MANUFACTURERS ADDRESS: 2411 Garden Road, Monterey, CA, 93940, USA	
PLANT LOCATIONS:	
<b>CATEGORY OF FITTINGS TO BE REGISTERED. CIRCLE ONE CATEGORY ONLY</b> A Pipe fittings, including couplings, tees, elbows, Ys, plugs, unions, pipe caps, or reducers B Flanges all flanges C Valves all line valves D Expansion joints, flexible connections, and hose assemblies all types E Strainers, filters, separators, and steam traps F Measuring devices, including pressure gauges, level gauges, sight glasses, levels, or pressure transmitters G Certified capacity-rated pressure relief devices acceptable as primary over pressure protection on boilers, pressure vessels, piping and fusible plugs H Pressure retaining components that do not fall into one of the above categories N Nuclear components Class 1 <input type="checkbox"/> Class 2 <input type="checkbox"/> Class 3 <input type="checkbox"/> (Meeting CNSC or ASME requirements)	<b>TITLE OF THE STANDARD OF CONSTRUCTION</b>  ASME B31.3 2012 EDITION
<b>SHOW MANUFACTURERS NAME, TRADEMARK, OR LOGO AS IT WILL APPEAR ON THE PRODUCT</b>  	
<b>TYPE OF CONSTRUCTION</b> FORGED <input type="checkbox"/> WELDED <input checked="" type="checkbox"/> WROUGHT <input type="checkbox"/> CAST <input type="checkbox"/> OTHER <input type="checkbox"/> DESCRIBE OTHER:	
<b>LIST OF SUPPORTING DOCUMENTATION AND IDENTIFICATION OF THE ACTUAL ITEMS TO BE REGISTERED:</b>  PVEscp-8217-1  Series 45-1FTB Insertion Mass Flow Transmitters	

## DECLARATION:

I, Daniel Kurz, being employed by Kurz Instruments and being the person having full authority and responsibility for the quality of the end product do solemnly declare that the information contained in this form is true and to the best of my knowledge represents the product for which registration is sought. The dimensions, materials of construction, pressure temperature ratings, and identification markings are in accordance with the herein named standards. I further declare that the manufacture of these fittings is regulated by a Quality Control Program which extends to each plant where fabrication occurs in whole or in part and has been verified by FM Approvals as being suitable for that purpose and I make this solemn declaration conscientiously believing it to be true, and knowing that it is of the same force and effect as if made under oath.


Signature of Declarant: [Signature]

Declared before me at Monterey County, California

This 25 day of June AD 2014

Commissioner of Oaths  
or Notary Public (sign)

[Signature]

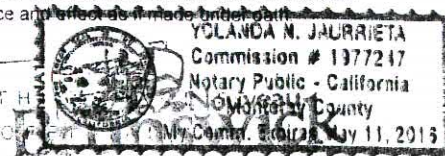

DEPT OF PUBLIC SAFETY  
BOILER & PRESSURE VESSEL ACT

This space for Regulatory Authority use This registration must be revalidated after ten (10) years from the date of registration	
CRN: <u>0F06882.2 Add.1</u> FID#: <u>2013</u>	<b>REGISTRATION ONLY</b> CRN <u>0F06882.27 Add.1</u> EXAMINER: <u>[Signature]</u> for <b>CHIEF BOILER INSPECTOR</b> DATE: <u>10/3/2014</u>
<b>NOTES:</b> 1. All fittings shall be registered in the name of the Manufacturer. 2. Each category shall be supported with two Statutory Declaration forms and one copy of supporting documentation. 3. The declaration shall be made by the person having full authority and responsibility for the quality of the end product. 4. Quality control programs shall be resubmitted for validation at a maximum interval of five (5) years.	<input type="checkbox"/> B.P.s <input type="checkbox"/> P.V.s Sect. 10 - Fittings Rev. 1/05/2003 <input type="checkbox"/> FITTINGS <input type="checkbox"/> COMPONENTS


# UNIFORM STATUTORY DECLARATION FORM FOR THE REGISTRATION OF FITTING DESIGNS

NEW BRUNSWICK  
NUNAVUT

NOVA SCOTIA  
YUKON


PRINCE EDWARD ISLAND  
NORTHWEST TERRITORIES

NEWFOUNDLAND AND LABRADOR

MANUFACTURERS NAME: Kurz Instruments	
MANUFACTURERS ADDRESS: 2411 Garden Road, Monterey, CA, 93940, USA	
PLANT LOCATIONS:	
<p><b>CATEGORY OF FITTINGS TO BE REGISTERED. CIRCLE ONE CATEGORY ONLY</b></p> <p>A Pipe fittings, including couplings, tees, elbows, Ys, plugs, unions, pipe caps, or reducers</p> <p>B Flanges: all flanges</p> <p>C Valves: all line valves</p> <p>D Expansion joints, flexible connections, and hose assemblies: all types</p> <p>E Strainers, filters, separators, and steam traps</p> <p>F Measuring devices, including pressure gauges, level gauges, sight glasses, levels, or pressure transmitters</p> <p>G Certified capacity-rated pressure relief devices acceptable as primary over pressure protection on boilers, pressure vessels, piping and fusible plugs</p> <p>H Pressure retaining components that do not fall into one of the above categories</p> <p>N Nuclear components: Class 1 <input type="checkbox"/> Class 2 <input type="checkbox"/> Class 3 <input type="checkbox"/> (Meeting CNSC or ASME requirements)</p>	<p><b>TITLE OF THE STANDARD OF CONSTRUCTION</b></p> <p>ASME B31.3 2012 EDITION</p>
<p><b>SHOW MANUFACTURERS NAME, TRADEMARK, OR LOGO AS IT WILL APPEAR ON THE PRODUCT</b></p> 	<p><b>TYPE OF CONSTRUCTION</b></p> <p>FORGED <input type="checkbox"/> WELDED <input checked="" type="checkbox"/> WROUGHT <input type="checkbox"/></p> <p>CAST <input type="checkbox"/> OTHER <input type="checkbox"/></p> <p>DESCRIBE OTHER:</p>
<p><b>LIST OF SUPPORTING DOCUMENTATION AND IDENTIFICATION OF THE ACTUAL ITEMS TO BE REGISTERED:</b></p> <p>PVEscp-8217-1</p> <p>Series 454FTB Insertion Mass Flow Transmitters</p>	

## DECLARATION:


I, Daniel Kurz, (hereinafter employed by Kurz Instruments) and being the person having full authority and responsibility for the quality of the end product do solemnly declare that the information contained in this form is true and to the best of my knowledge represents the product for which registration is sought. The dimensions, materials of construction, pressure temperature ratings, and identification markings are in accordance with the herein named standards. I further declare that the manufacture of these fittings is regulated by a Quality Control Program which extends to each plant where fabrication occurs in whole or in part and has been verified by FM Approvals as being suitable for that purpose and I make this solemn declaration conscientiously believing it to be true, and knowing that it is of the same force and effect as if made under oath.


Signature of Declarer: 


Declared before me at Monterey County, California on the 25 day of June AD 2014

This 25 day of June AD 2014

Commissioner of Oaths

or Notary Public (Sign): 

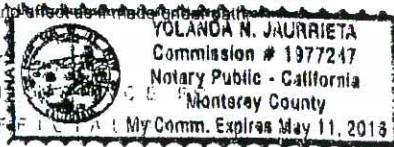

This space for Regulatory Authority use	
This registration must be revalidated after ten (10) years from the date of acceptance.	
CRN: <u>OF06882.2 Add.1</u>	<p>Newfoundland Labrador Service NL</p> <p>Registered <u>OF06882.2 Add.1</u></p> <p>Date <u>14/10/03</u></p> <p>Engineering and Inspection Services</p> <p>Registered by </p> <p>UNDER THE AUTHORITY OF THE PUBLIC SAFETY ACT AND THE BOILER, PRESSURE VESSEL AND COMPRESSED GAS REGULATIONS</p>
FID#: <u>2013</u>	
Notes:	
<p>1. All fittings shall be registered in the name of the Manufacturer.</p> <p>2. Each category shall be supported with two Statutory Declaration forms and one copy of supporting documentation.</p> <p>3. The declaration shall be made by the person having full authority and responsibility for the quality of the end product.</p> <p>4. Quality control programs shall be resubmitted for validation at a maximum interval of five (5) years.</p>	




# UNIFORM STATUTORY DECLARATION FORM FOR THE REGISTRATION OF FITTING DESIGNS

NEW BRUNSWICK  
NUNAVUT

NOVA SCOTIA  
YUKON

PRINCE EDWARD ISLAND  
NORTHWEST TERRITORIES

NEWFOUNDLAND AND LABRADOR

MANUFACTURERS NAME: Kurz Instruments	
MANUFACTURERS ADDRESS: 2411 Garden Road, Monterey, CA, 93940, USA	
PLANT LOCATIONS:	
<p><b>CATEGORY OF FITTINGS TO BE REGISTERED. CIRCLE ONE CATEGORY ONLY</b></p> <p>A Pipe fittings, including couplings, tees, elbows, Ys, plugs, unions, pipe caps, or reducers</p> <p>B Flanges: all flanges</p> <p>C Valves: all line valves</p> <p>D Expansion joints, flexible connections, and hose assemblies: all types</p> <p>E Strainers, filters, separators, and steam traps</p> <p>F Measuring devices, including pressure gauges, level gauges, sight glasses, levels, or pressure transmitters</p> <p>G Certified capacity-rated pressure relief devices acceptable as primary over pressure protection on boilers, pressure vessels, piping and fusible plugs</p> <p>H Pressure retaining components that do not fall into one of the above categories</p> <p>N Nuclear components: Class 1 <input type="checkbox"/> Class 2 <input type="checkbox"/> Class 3 <input type="checkbox"/> (Meeting CNSC or ASME requirements)</p>	<p><b>TITLE OF THE STANDARD OF CONSTRUCTION</b></p> <p>ASME B31.3 2012 EDITION</p>
<p><b>SHOW MANUFACTURERS NAME, TRADEMARK, OR LOGO AS IT WILL APPEAR ON THE PRODUCT</b></p> 	<p><b>TYPE OF CONSTRUCTION</b></p> <p>FORGED <input type="checkbox"/> WELDED <input checked="" type="checkbox"/> WROUGHT <input type="checkbox"/></p> <p>CAST <input type="checkbox"/> OTHER <input type="checkbox"/></p> <p>DESCRIBE OTHER:</p>
<p><b>LIST OF SUPPORTING DOCUMENTATION AND IDENTIFICATION OF THE ACTUAL ITEMS TO BE REGISTERED:</b></p> <p>PVEscp-8217-1</p> <p>Series 454FTB Insertion Mass Flow Transmitters</p>	

## DECLARATION:


I, Daniel Kurz, (signature) employed by Kurz Instruments and being the person having full authority and responsibility for the quality of the end product do solemnly declare that the information contained in this form is true and to the best of my knowledge represents the product for which registration is sought. The dimensions, materials of construction, pressure temperature ratings, and identification markings are in accordance with the herein named standards. I further declare that the manufacture of these fittings is regulated by a Quality Control Program which extends to each plant where fabrication occurs in whole or in part and has been verified by FM Approvals as being suitable for that purpose and I make this solemn declaration conscientiously believing it to be true, and knowing that it is of the same force and effect as made under oath.

Signature of Declarer: [Signature]

Declared before me at Monterey County, California on the 25 day of June AD 2014

This 25 day of June AD 2014

Commissioner of Oaths  
or Notary Public: (sign) [Signature]

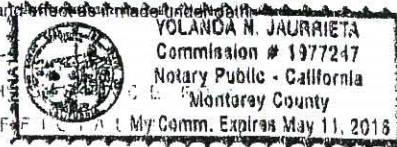

<p>This space for Regulatory Authority use</p> <p>This registration must be revalidated after ten (10) years from the date of acceptance</p>	
CRN: <u>0F06882.2 Add.1</u>	
FID#: <u>2013</u>	
<p><b>Notes</b></p> <p>1. All fittings shall be registered in the name of the Manufacturer.</p> <p>2. Each category shall be supported with two Statutory Declaration forms and one copy of supporting documentation.</p> <p>3. The declaration shall be made by the person having full authority and responsibility for the quality of the end product.</p> <p>4. Quality control programs shall be resubmitted for validation at a maximum interval of five (5) years.</p>	
<p>Sect. 1.0 - Fittings Rev. 1/05/2003</p>	




# UNIFORM STATUTORY DECLARATION FORM FOR THE REGISTRATION OF FITTING DESIGNS

NEW BRUNSWICK  
NUNAVUT

NOVA SCOTIA  
YUKON

PRINCE EDWARD ISLAND  
NORTHWEST TERRITORIES

NEWFOUNDLAND AND LABRADOR

MANUFACTURERS NAME: Kurz Instruments	
MANUFACTURERS ADDRESS: 2411 Garden Road, Monterey, CA, 93940, USA	
PLANT LOCATIONS:	
<p><b>CATEGORY OF FITTINGS TO BE REGISTERED. CIRCLE ONE CATEGORY ONLY</b></p> <p>A Pipe fittings, including couplings, tees, elbows, Ys, plugs, unions, pipe caps, or reducers</p> <p>B Flanges: all flanges</p> <p>C Valves: all line valves</p> <p>D Expansion joints, flexible connections, and hose assemblies: all types</p> <p>E Strainers, filters, separators, and steam traps</p> <p>F Measuring devices, including pressure gauges, level gauges, sight glasses, levels, or pressure transmitters</p> <p>G Certified capacity-rated pressure relief devices acceptable as primary over pressure protection on boilers, pressure vessels, piping and fusible plugs</p> <p>H Pressure retaining components that do not fall into one of the above categories</p> <p>N Nuclear components: Class 1 <input type="checkbox"/> Class 2 <input type="checkbox"/> Class 3 <input type="checkbox"/> (Meeting CNSC or ASME requirements)</p>	<p><b>TITLE OF THE STANDARD OF CONFORMANCE</b></p> <p>ASME B31.3 2012 EDITION</p>
<p><b>SHOW MANUFACTURERS NAME, TRADEMARK, OR LOGO AS IT WILL APPEAR ON THE PRODUCT</b></p> 	<p><b>TYPE OF CONSTRUCTION</b></p> <p>FORGED <input type="checkbox"/> WELDED <input checked="" type="checkbox"/> WROUGHT <input type="checkbox"/></p> <p>CAST <input type="checkbox"/> OTHER <input type="checkbox"/></p> <p>DESCRIBE OTHER:</p>
<p><b>LIST OF SUPPORTING DOCUMENTATION AND IDENTIFICATION OF THE ACTUAL ITEMS TO BE REGISTERED:</b></p> <p>PVEscp-8217-1</p> <p>Series 454FTB Insertion Mass Flow Transmitters</p>	

## DECLARATION:


I, Daniel Kurz, (hereinafter employed by Kurz Instruments) and being the person having full authority and responsibility for the quality of the end product do solemnly declare that the information contained in this form is true and to the best of my knowledge represents the product for which registration is sought. The dimensions, materials of construction, pressure temperature ratings, and identification markings are in accordance with the herein named standards. I further declare that the manufacture of these fittings is regulated by a Quality Control Program which extends to each plant where fabrication occurs in whole or in part and has been verified by FM Approvals as being suitable for that purpose and I make this solemn declaration conscientiously believing it to be true, and knowing that it is of the same force and effect as if made by me.

Signature of Declarer: [Signature]

Declared before me at Monterey County, California on the 25 day of June AD 2014

This 25 day of June AD 2014

Commissioner of Oaths  
or Notary Public (Sign): [Signature]

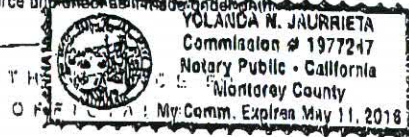

<p>This space for Regulatory Authority use</p> <p>This registration must be revalidated after ten (10) years from the date of acceptance.</p>	
C.R.N. <u>0F06882.2 Add.1</u>	<p>Northwest Territories</p> <p><b>REGISTERED</b></p> <p>UNDER THE AUTHORITY OF THE BOILER AND PRESSURE VESSEL ACT.</p> <p>C.R.N. <u>0F06882.2 T Add.1</u></p> <p>SIGNED <u>[Signature]</u></p> <p>DATE <u>06/14/2014</u></p>
FID#: <u>2013</u>	
Notes:	
<p>1. All fittings shall be registered in the name of the Manufacturer.</p> <p>2. Each category shall be supported with two Statutory Declaration forms and one copy of supporting documentation.</p> <p>3. The declaration shall be made by the person having full authority and responsibility for the quality of the end product.</p> <p>4. Quality control programs shall be resubmitted for validation at a maximum interval of five (5) years.</p>	

158.00


# **UNIFORM STATUTORY DECLARATION FORM FOR THE REGISTRATION OF FITTING DESIGNS**

NEW BRUNSWICK  
NUNAVUT

NOVA SCOTIA  
YUKON

PRINCE EDWARD ISLAND  
NORTHWEST TERRITORIES

NEWFOUNDLAND AND LABRADOR

MANUFACTURERS NAME: Kurz Instruments	
MANUFACTURERS ADDRESS: 2411 Garden Road, Monterey, CA, 93940, USA	
PLANT LOCATIONS:	
<b>CATEGORY OF FITTINGS TO BE REGISTERED. CIRCLE ONE CATEGORY ONLY</b> A Pipe fittings, including couplings, tees, elbows, Ys, plugs, unions, pipe caps, or reducers B Flanges: all flanges C Valves: all line valves D Expansion joints, flexible connections, and hose assemblies: all types E Strainers, filters, separators, and steam traps F Measuring devices, including pressure gauges, level gauges, sight glasses, levels, or pressure transmitters G Certified capacity-rated pressure relief devices acceptable as primary over pressure protection on boilers, pressure vessels, piping and fusible plugs H Pressure retaining components that do not fall into one of the above categories N Nuclear components: Class 1 <input type="checkbox"/> Class 2 <input type="checkbox"/> Class 3 <input type="checkbox"/> (Meeting CNSC or ASME requirements)	<b>TITLE OF THE STANDARD OF CONSTRUCTION</b> ASME B31.3 2012 EDITION
<b>SHOW MANUFACTURERS NAME, TRADEMARK, OR LOGO AS IT WILL APPEAR ON THE PRODUCT</b> 	<b>TYPE OF CONSTRUCTION</b> FORGED <input type="checkbox"/> WELDED <input checked="" type="checkbox"/> WROUGHT <input type="checkbox"/> CAST <input type="checkbox"/> OTHER <input type="checkbox"/> DESCRIBE OTHER:
<b>LIST OF SUPPORTING DOCUMENTATION AND IDENTIFICATION OF THE ACTUAL ITEMS TO BE REGISTERED:</b> PVEscp 8217-1 Series 454F13 Insertion Mass Flow Transmitters	


**DECLARATION:**

I, Daniel Kurz (see note 1) employed by Kurz Instruments and being the person having full authority and responsibility for the quality of the end product do solemnly declare that the information contained in this form is true and to the best of my knowledge represents the product for which registration is sought. The dimensions, materials of construction, pressure temperature ratings, and identification markings are in accordance with the herein named standards. I further declare that the manufacture of these fittings is regulated by a Quality Control Program which extends to each plant where fabrication occurs in whole or in part and has been verified by FM Approvals as being suitable for that purpose and I make this solemn declaration conscientiously believing it to be true, and knowing that it is of the same force and effect as if made under oath.

Signature of Declarer: [Signature]

Declared before me at Monterey County, California on the 25 day of June AD 2014

Commissioner of Oaths  
or Notary Public (sign): [Signature]

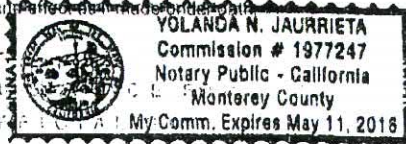

This space for Regulatory Authority Use This registration must be revalidated after ten (10) years from the date of acceptance.	
CRN: <u>0F06882.2 Add.1</u> RID#: <u>2013</u>	<b>NUNAVUT</b> Boilers and Pressure Vessels Act <b>REGISTERED</b> CRN <u>0F06882.2NAdd1</u> Date <u>OCT 14 2014</u> Signed <u>[Signature]</u> <small>Sect. 4.0, Fittings Rev. 1 06/2003</small> Chief Inspector
<b>Notes</b> 1. All fittings shall be registered in the name of the Manufacturer. 2. Each category shall be supported with two Statutory Declaration forms and one copy of supporting documentation. 3. The declaration shall be made by the person having full authority and responsibility for the quality of the end product. 4. Quality control programs shall be resubmitted for validation at a maximum interval of five (5) years.	<b>Territorial Registration Fee</b>



2202 2nd Avenue  
Regina, SK S4R 1K3  
Canada

306-787-1443  
info@tsask.ca  
www.tsask.ca

## REGISTRATION APPROVAL

Tuesday, January 06, 2015

Pressure Vessel Engineering Ltd.  
120 Randall Drive, Suite B  
Waterloo, ON  
N2V 1C6

**ATTENTION :** Catherine Diplock

**Our File :** 9578 [ 0 F


With reference to your submission respecting the registration of the item below, for legal use in the province, please note we have surveyed, approved and registered this design as noted.

MANUFACTURER :		Kurz Instruments, Inc.	
CATALOG OR DRAWING : Brochure 454FTB			
ITEM : Series 454FTB Mass Flow Transmitter		CRN :	OF06882.23

We wish to point out that every fitting must be constructed strictly in accordance with the registered design.

Fitting registrations are required to be resubmitted for validation after ten (10) years from the registration date in accordance with CSA B51, Clause 4.2.1. The date of expiry for this registration is **Aug 28, 2024**

Sincerely,




Kalam Azad, P.Eng.

Codes and Standards Compliance

**REMARKS:** CRN registered under reciprocal agreement.



# Technical Safety Authority of Saskatchewan

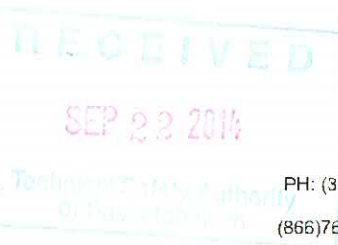

2202 2nd Ave.  
Regina, SK S4R 1K3  
PH: (306)798-7112 Toll Free: (866)530-8599  
FAX: (306)787-9273 Toll Free:  
(866)760-9255 Email: [boilerpermits@tsask.ca](mailto:boilerpermits@tsask.ca)  
Website: [www.tsask.ca](http://www.tsask.ca)

## Statutory Declaration (Registration of Filings)

TSK-1008

### I. Declaration Information

I, Daniel Kurz  
General Manager  
(company title, e.g. vice president, plant manager, chief engineer)  
(must be in a position of authority in the manufacturing plant where the fitting is produced)  
of: Kurz Instruments  
(name of manufacturer)

In this space, show facsimile of  
manufacturer's logo or trademark as it will  
appear on the fitting.



located at: 2411 Garden Road, Monterey, CA, 93940, USA  
(Plant Address - Apt/Street) (City, Prov) (Postal Code)

do solemnly declare that the fittings listed hereinunder, which are subject to the **Saskatchewan Boiler and Pressure Vessel Safety Act** (check one)

- ☐ Comply with the requirements of \_\_\_\_\_ which specifies the dimensions,  
(title of recognized North American Standard)  
Materials of construction, pressure / temperature ratings and identification marking of the fittings, or
- ☒ Are not covered by the provisions of a recognized North American standard and are therefore manufactured  
to comply with ASME B31.3 2012 EDITION as supported by the attached  
data which identifies the dimensions, materials of construction, pressure / temperature ratings and the basis  
for such ratings, and the marking of the fittings for identification.

I further declare that the manufacturer of these fittings is controlled by a quality control program which has been  
verified by the following authority, FM Approvals as being suitable for the manufacturer  
of these fittings to the stated standard. The fittings covered by this declaration, for which I seek registration, are  
Series 454FTB Insertion Mass Flow Transmitters

In support of this application, the following information, calculations and / or test data are attached:

PVEscp-8217-1



### II. Declaration

DECLARED before me at California In the County of Monterey  
this 25 day of June, 2014  
Yolanda N Saurrieta (print name) \_\_\_\_\_ (Signature)  
Yolanda N Saurrieta (Signature of Commissioner of Oaths)

### III. Office Use Only

To the best of my knowledge and belief, the application meets the requirements of the **Boiler and Pressure Vessel Safety Act** and  
CSA B51, Clause 4.2, and is accepted for registration in Category \_\_\_\_\_

(Registration Number)

(Date Registered - MM DD YYYY)

(Expiry Date - MM DD YYYY)

(For the Administrator / Chief Inspector)





# Kurz Instruments - Series 454FTB Insertion Mass Flow Transmitters

## PVEscp-8217-1.0

This submission is a re-registration of fittings using CSA B51-14 Part 1 4.2.8(c) method.

The current registration uses the exact pressure retaining components of the previous CRN registration 0F06882.2

Model Number

454FTB-08-MT	Flange Size	316 SS SA-240 316L Plate	304 SS SA-240 304L Plate	Hastalloy C276 SB-575 Alloy N10276	Monel SB-127 Alloy N04400
	1/2" Class 150	YES	YES	YES	YES
	1/2" Class 300	YES	YES	YES	YES
	3/4" Class 150	YES	YES	YES	YES
	3/4" Class 300	YES	YES	YES	YES
	1" Class 150	YES	YES	YES	YES
	1" Class 300	YES	YES	YES	YES
	1-1/2" Class 150	YES	YES	YES	YES
	1-1/2" Class 300	YES	YES	YES	YES
	2" Class 150	YES	YES	YES	YES
	2" Class 300	YES	YES	YES	YES
	3" Class 150	YES	YES	YES	YES
	3" Class 300	YES	YES	YES	YES
	4" Class 150	YES	YES	YES	YES
	4" Class 300	YES	YES	YES	YES

454FTB-08-HHT	Flange Size	316 SS SA-240 316L Plate	304 SS SA-240 304L Plate	Hastalloy C276 SB-575 Alloy N10276	Monel SB-127 Alloy N04400
	1/2" Class 150	NO	NO	YES	YES
	1/2" Class 300	NO	NO	YES	YES
	3/4" Class 150	NO	NO	YES	YES
	3/4" Class 300	NO	NO	YES	YES
	1" Class 150	NO	NO	YES	YES
	1" Class 300	NO	NO	YES	YES
	1-1/2" Class 150	NO	NO	YES	YES
	1-1/2" Class 300	NO	NO	YES	YES
	2" Class 150	NO	NO	YES	YES
	2" Class 300	NO	NO	YES	YES
	3" Class 150	NO	NO	YES	YES
	3" Class 300	NO	NO	YES	YES
	4" Class 150	NO	NO	YES	YES
	4" Class 300	NO	NO	YES	YES

Technical Safety Authority  
of Saskatchewan  
Boiler & P.V. Safety Unit

CRN 0F 06882.2  
File 9578

REGISTERED

Date 06 Jun 2015

Expiry 28 Aug 2024  
Design Survey Office

454FTB-12-MT	Flange Size	316 SS SA-240 316L Plate	304 SS SA-240 304L Plate	Hastalloy C276 SB-575 Alloy N10276	Monel SB-127 Alloy N04400
	3/4" Class 150	YES	YES	YES	YES
	3/4" Class 300	YES	YES	YES	YES
	1" Class 150	YES	YES	YES	YES
	1" Class 300	YES	YES	YES	YES
	1-1/2" Class 150	YES	YES	YES	YES
	1-1/2" Class 300	YES	YES	YES	YES

454FTB-12-HHT	Flange Size	316 SS SA-240 316L Plate	304 SS SA-240 304L Plate	Hastalloy C276 SB-575 Alloy N10276	Monel SB-127 Alloy N04400
	3/4" Class 150	NO	NO	YES	YES
	3/4" Class 300	NO	NO	YES	YES
	1" Class 150	NO	NO	YES	YES
	1" Class 300	NO	NO	YES	YES
	1-1/2" Class 150	NO	NO	YES	YES
	1-1/2" Class 300	NO	NO	YES	YES

454FTB-16-MT	Flange Size	316 SS SA-240 316L Plate	304 SS SA-240 304L Plate	Hastalloy C276 SB-575 Alloy N10276	Monel SB-127 Alloy N04400
	1" Class 150	YES	YES	YES	YES
	1" Class 300	YES	YES	YES	YES
	1-1/2" Class 150	YES	YES	YES	YES
	1-1/2" Class 300	YES	YES	YES	YES
	2" Class 150	YES	YES	YES	YES
	2" Class 300	YES	YES	YES	YES
	3" Class 150	YES	YES	YES	YES
	3" Class 300	YES	YES	YES	YES
	4" Class 150	YES	YES	YES	YES
	4" Class 300	YES	YES	YES	YES

454FTB-16-HHT	Flange Size	316 SS SA-240 316L Plate	304 SS SA-240 304L Plate	Hastalloy C276 SB-575 Alloy N10276	Monel SB-127 Alloy N04400
	1" Class 150	NO	NO	YES	YES
	1" Class 300	NO	NO	YES	YES
	1-1/2" Class 150	NO	NO	YES	YES
	1-1/2" Class 300	NO	NO	YES	YES
	2" Class 150	NO	NO	YES	YES
	2" Class 300	NO	NO	YES	YES
	3" Class 150	NO	NO	YES	YES
	3" Class 300	NO	NO	YES	YES
	4" Class 150	NO	NO	YES	YES
	4" Class 300	NO	NO	YES	YES



PVE-8217: Kurz Instruments Inc. – Series 454FTB Insertion Mass Flow Transmitters

Monday, July 07, 2014

Dear Reviewer,

Our customer, Kurz Instruments Inc. would like to apply for CRN re-registration using CSA B51-14 Part 1 4.2.8 (c ) methods for their series 454FTB Insertion Mass Flow Transmitters. There are a few items of note that may assist you with the review process.

The current re-registration submission is an exact duplicate (uses same pressure retaining components) of the previous CRN registration ~~0F67882.2~~. The scope of the registration remains the same between the original submission and the re-registration.

*0F06882.2*

Please find the following documentation included in this submission package:

- Statutory Declaration – Signed and Notarized Statutory Declaration.
- Scope of project – PVEscp-8217-1.0
- Product Catalogue – Series 454FTB Insertion Mass Flow Transmitters
- Manufacturers QC – ISO 9001:2008

If you have any question please contact me.

Regards,



Kevin Myers  
Pressure Vessel Engineering Ltd.  
519-880-9808 x 246

**ABSA**  
the pressure equipment safety authority  
**STATUTORY DECLARATION**  
Registration of Fittings

In this space, show facsimile of  
manufacturer's logo or  
trademark as it will appear on  
the fitting.




I, Daniel Kurz,

General Manager

(company title, e.g. vice president, plant manager, chief engineer) (must be in a position of authority)

of Kurz Instruments  
(name of manufacturer)

located at 2411 Garden Road, Monterey, CA, 93940, USA  
(plant address)

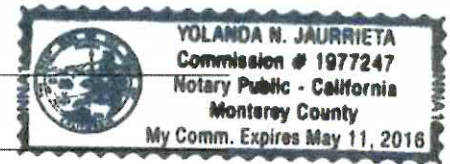

do solemnly declare that the fittings listed hereunder, which are subject to the Safety Codes Act  
(check one)

- ☐ comply with the requirements of \_\_\_\_\_ which specifies the dimensions,  
(title of recognized North American Standard)  
materials of construction, pressure/temperature ratings and identification marking of the fittings, or
- ☒ are not covered by the provisions of a recognized North American standard and are therefore manufactured to  
comply with ASME B31.3 2012 EDITION as supported by the attached data which identifies the dimensions,  
materials of construction, pressure/temperature ratings and the basis for such ratings, and the marking of the fittings  
for identification.

I further declare that the manufacture of these fittings is controlled by a quality control program which has been verified by the  
following authority, FM Approvals as being suitable for the manufacture of these fittings to the  
stated standard. The fittings covered by this declaration, for which I seek registration, are Series 454FTB Insertion Mass Flow  
Transmitters  
In support of this application, the following information, calculations and/or test data are attached:

PVEscp-8217-1

DECLARED before me at California in the County of Monterey  
this 25 day of June, 2014  
(Month) (Year)  
(print) Yolanda N. Jaurrieta  
(sign) Yolanda N. Jaurrieta  
(A Commissioner for Oaths)

[Signature]  
(Signature of Applicant)

**For Office Use Only**

To the best of my knowledge and belief, the application meets the requirements of the Safety Codes Act and CSA Standard  
B51, Clause 4.2, and is accepted for registration in Category F

Registration Number OF 06882 2

Date Registered: AUG 28 2014

[Signature]  
(For the Administrator/Chief Inspector of Alberta)

Expiry Date: August 28, 2014

The information you provide is necessary only for the administration of the programs as required by the Alberta Safety Codes Act and Regulations in the Boiler Discipline.



August 28, 2014

**Attention:** Catherine Diplock  
PRESSURE VESSEL ENGINEERING INC  
120 RANDALL DRIVE SUITE B  
WATERLOO, ON N2V 1C6

The design submission, tracking number 2014-05500, originally received on July 09, 2014 was surveyed and accepted for registration as follows:

**CRN :** 0F06882.2

**Accepted on:** August 28, 2014

**Reg Type:** Addition to Acc. Fitting

**Expiry Date:** August 28, 2024

**Drawing No. :** PVESCP-8217-1.0

**Fitting type:** SERIES 454FTB MASS FLOW TRANSMITTERS

Design registered in the name of : KURZ INSTRUMENTS

**The registration is conditional on your compliance with the following notes:**

*The CRN renewal is given based on the understanding that there is no change to the originally registered design.*

*This registration is valid only for fittings fabricated at the location(s) covered by the QC certificate attached to the accepted AB-41 Statutory Declaration form. This registration is valid only until the indicated expiry date only if the Manufacturer maintains a valid quality management system approved by an acceptable third-party agency until that date. Should the approval of the quality management system lapse before the expiry date indicated above, this registration shall become void.*

An invoice covering survey and registration fees will be forwarded from our Revenue Accounts.

Enclosed are stamped prints for your reference.

Sincerely,



ONSHCHENKO, TETYANA, P. Eng.



SERIES 454FTB

SINGLE-POINT INSERTION  
THERMAL MASS FLOW  
TRANSMITTERS



REVISION

OF 06882.26

28 NOV. 2014

*hb*

**KURZ**  
INSTRUMENTS INC.

CE



**HART**  
COMMUNICATION PROTOCOL



**DESCRIPTION**

The Series 454FTB represents the Kurz family of state-of-the-art microprocessor based, industrial quality, Single-Point Insertion Mass Flow Transmitters for industrial gases.

The 454FTB includes the most advanced temperature compensation, microprocessor technology and the highest repeatability, accuracy, and reliability available. It has many improvements and features that greatly enhance the performance including, the FD2-HT sensor rated at 260°C, electronic self-check functions, a flow control valve PID controller, a patented digital thermal anemometer bridge, a more convenient remote electronic mounting configuration, a single PCB for improved reliability and ease-of-use, built-in sensor cleaning purge timer, external inputs/outputs, and many other Kurz engineering and functional features.

The 454FTB has CE Compliance and a Canadian Registration Number for most applications. The 454FTB meets CSA (USA and Canada), IECEx and ATEX Non-Incendive and Explosion-Proof/Flame-Proof Safety Standards and are Type 4, IP66 rated. Kurz is an ISO 9001 Quality Manufacturer.

**KEY FEATURES**

- Constant temperature sensor control circuit.
- Fastest response to temperature and velocity changes in the industry.
- Sensors and electronics (single PCB) are interchangeable. No matched sets.
- 3-year warranty. All components pass an extensive accelerated stress test for high reliability.
- Velocity dependent correction factors for flow rate.
- Velocity-Temperature Mapping (VTM) for wide ranging velocity and temperature.
- Zero velocity is a valid data point.
- Built-in Zero-Mid-Span CEMS electronics drift check circuits.
- Automatic Sensor Blockage Correction Factor (SBCF).
- Built-in flow totalizers and elapsed time.
- PID flow controller.
- Process temperature rating from -40°C to +260°C (HT) or from -40°C to +500°C (HHT).
- Electronics operating temperature range from -40°C to +65°C, non-condensing.
- Process pressure rating up to 300 PSIG.
- Velocity range of 0-24,000 SFPM (112 NMPS).
- Input power options of 85 to 265 VAC 47/63 Hz or 24 VDC.
- Sensor lead length independent circuitry.
- Alloy C-276 all-welded sensor construction.
- Integral or remote electronics enclosure.
- Dual-chamber, polyester powder-coated aluminum (Type 4, IP66) electronics enclosure.
- Adjustable LCD/keypad orientation allows viewing the display in horizontal or vertical installations.
- Insensitive to orientation.
- Two optically-isolated, loop-powered 4-20 mA outputs (user configurable). Typically, one is configured for mass flow rate or mass velocity and the other for process temperature or for PID application (flow transmitters with the HART communication option have only one 4-20mA output).
- Easy-to-use menus for display and configuration.
- User-configurable scrolling or static displays of flow process variables.
- User selected English or Metric units (SFPM, SCFM, SCFH, PPM, PPH, °F; SMPS, NMPS, NLPM, NCMH, SLPM, SCMh, KGM, KGH, °C).
- User can change STP reference condition without affecting factory calibration data.
- Programmable alarm functions.
- User-selectable digital filtering.
- User programmable access codes.
- USB port for terminal operation.
- Modbus ASCII or RTU communications.
- Configuration upload/download software using a PC with USB connection, RS-485, or TCP/IP Modbus.
- Built-in purge timer and "hold value" feature during purge for use with Model 146 Sensor Cleaning System.
- Air Purge Sensor Cleaning System (optional).
- One 4-20mA input (optional).
- Two optically-isolated solid-state alarm/relays (optional).
- Two digital inputs dedicated to Purge and Zero-Mid-Span Drift Check (optional).
- Pulsed output for use as a remote flow totalizer (optional).
- HART 7 communication (optional).
- 4-20 mA outputs meet NAMUR NE43 recommendations.
- Meets EPA mandatory GHG Certification requirement in CFR98.34(c)(1).
- CE compliance including EMC, ATEX, LVD, PED, WEEE and ROHS EU directives.
- Non-Incendive and Explosion-Proof/Flame-Proof Safety Approvals (CSA/ATEX/IECEX).

**APPLICATIONS**

- Industrial and process gas mass flows
- Combustion air flow measurements
- EPA flow monitors
- Flare stack metering
- Aeration air flow
- Incinerator stack mass flow
- Solvent recovery system mass flow
- VOC mass flow
- Cement plants
- Coal-fired boiler combustion air
- Compressed air
- Natural gas, and most industrial gases
- Semi-conductor processing gas metering
- Nuclear power plants
- Air sampling in DOE facilities
- OEM applications

**OUR MISSION**

To manufacture and market the best thermal mass flow meters available and to support our customers in their efforts to improve their business.



# SERIES 454FTB SINGLE-POINT INSERTION THERMAL MASS FLOW TRANSMITTERS

## PRINCIPLE OF OPERATION

The Series 454FTB uses the well-recognized Kurz thermal convection mass flow measurement method by detecting the heat transfer from the heated RTD sensor ( $R_p$ ) referenced to the temperature of the ambient gas stream RTD sensor ( $R_{tc}$ ). A constant temperature difference between the heated sensor and the temperature sensor is maintained with a patented digital control circuit providing unexcelled speed of response and the many other advantages of constant temperature thermal anemometry. The microprocessor-based electronics measures the heat transfer, computes the standard velocity and ambient gas temperature, and allows the user to configure and set-up the 454FTB to fit all flow requirements. Display screens are easy-to-use and provide all the flow and temperature and diagnostic information. For a detailed description of Kurz technology, please see document number 364003, "Theory and Application of Kurz Thermal Convection Mass Flow Meters" by contacting Kurz or visiting our website.



Figure 1—Series 454FTB with LCD/Keypad Option

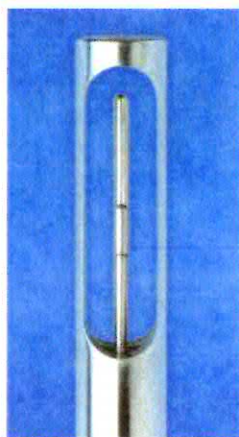


Figure 2—Fast Dual (FD2) Sensor

## CALIBRATION CURVE

Figure 3 shows the basic flow calibration curve is non-linear, having a non-zero output (live zero) at zero flow and a nearly constant percent of reading accuracy. Zero is a valid data point for a Kurz meter. The 454FTB electronics linearizes this non-linear calibration data.

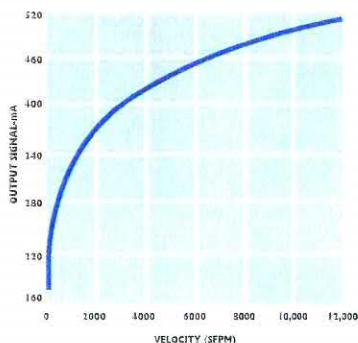


Figure 3—Calibration Curve

## TIME RESPONSE TO FLOW AND TEMPERATURE CHANGES

Figure 4 shows the response of a Kurz Fast Dual (FD2) MetalClad™ sensor to a step change in velocity. Kurz manufactures the fastest industrial quality sensors available.

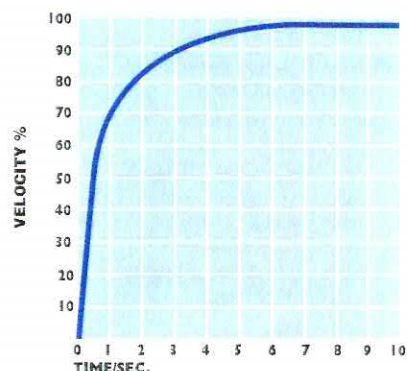


Figure 4—Sensor Flow Response

Figure 5 shows a typical response to a step change in temperature for a Kurz Fast Dual (FD2) MetalClad™ sensor. It is exceptional and allows use of the sensor for combustion air flow measurements in boilers that mix hot and cold air for temperature control (for example, in coal pulverizers).

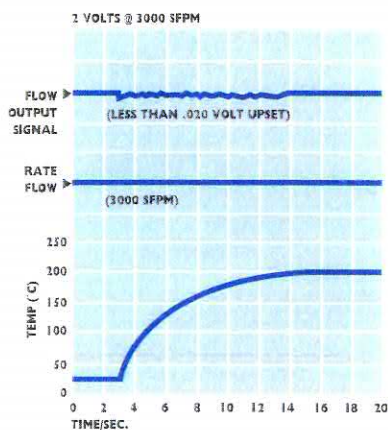


Figure 5—Sensor Temperature Response

## ORIENTATION EFFECTS

Figure 6 shows a typical output response to changes in the incoming velocity direction. Data is shown for rotation and yaw, as defined by Figure 7. Note that the effect is small for angles up to  $\pm 20$  degrees. This is extremely important for flow applications having severe turbulence and a non-axial velocity direction.

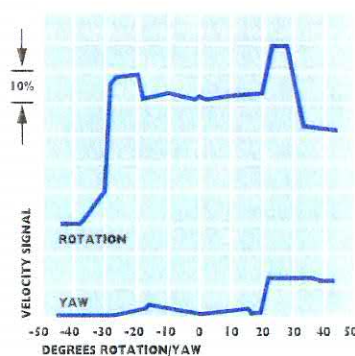


Figure 6—Sensor Measurement Error Versus Rotation/Yaw Angles




Figure 7—Sensor Rotation and Yaw Description



**SPECIFICATIONS**

**Process Temperature Rating:**

HT (-40°C to 260°C)  
HHT (-40°C to 500°C)

**Process Pressure Rating:**

300 PSIG (20 BARg)

**Sensor Material:** Alloy C-276;

optional abrasion-resistant Chromium Nitride coating on Alloy C-276 sensor materials. PTFE Compound coating for chemical resistance on Alloy C-276 sensor and sensor support. FD2 sensors, 260°C max

**Sensor Support Material:**

316L Stainless Steel, optional Alloy C-276

**Repeatability:** 0.25%

**Velocity Time Constant:**

1 second for velocity changes at 6000 SFPM at a constant temperature and 1 second for temperature changes at a constant velocity of 6000 SFPM

**Process Temperature**

**Time Constant:**

8 seconds at a velocity of 6000 SFPM

**Velocity Accuracy:**

See Feature 4 for overall accuracy including the effects of process temperature

**Temperature Accuracy:**

±(1/2% of reading + 1°C) for velocities above 100 SFPM

**Power:** +24 VDC ±10%, 85-265

VAC, 47/63 Hz; 24 watts max

**Enclosure Temperature**

**Rating:** -25°C to +65°C for all configurations; -40°C to +65°C for DC units without Display/Keypad

**Enclosures:** Polyester powder-coated aluminum, Type 4, IP66 with glass window for display option

**Solid-State Relays:**

Optically isolated, 0.5 ampere, 24 VAC/VDC maximum

**Analog Outputs (4-20 mA):**

Optically isolated, user loop-powered, 12-bit resolution and accuracy, maximum loop-resistance is 300 $\Omega$  at 18 VDC, 550 $\Omega$  at 24 VDC, 1400 $\Omega$  at 36 VDC; meets NAMUR NE43 recommendations

*Continued on next page*

**TECHNICAL DESCRIPTION**

**SENSOR DESIGN**

Series 454FTB Insertion Mass Flow Transmitters use the Kurz MetalClad™ FD2 all-welded Alloy C-276 sensor. In this design, the temperature sensor and velocity sensor are mounted in separate tubes (or stings), providing exceptional thermal isolation from the sensor support structure and fast response to process temperature changes.

**SENSOR MATERIALS AND CONSTRUCTION**

The standard sensor material for all Kurz metal sensors is Alloy C-276. This material is far superior to 316 Stainless Steel in high temperature and corrosive applications. Kurz offers Chromium Nitride coating for abrasive, dirty applications, such as in boiler coal pulverizers. Kurz exclusively uses Inconel sheathed mineral-insulated cable (MI cable) for temperatures above 260°C.

**PROCESS TEMPERATURE RATING**

Kurz offers sensor process temperature ratings of 260°C and 500°C. Field data verifies that the lifetime at 500°C is at least five years and the lifetime at 260°C is at least 10 years.

**TRANSMITTER CONFIGURATIONS**

Three available configurations: directly attached electronics enclosure, remote mount aluminum electronics enclosure, and remote wall-mount fiberglass electronics enclosure.

**PROCESS TEMPERATURE COMPENSATION**

The influence of temperature on the thermal properties of gases requires temperature compensation for repeatable and accurate measurements. Standard Temperature Compensation (STC) is used for applications in which the process temperature is below 125°C over a moderate velocity range or below 260°C over a more limited velocity range. If the process temperature and gas velocity vary widely, Velocity-Temperature Mapping (VTM) is recommended. VTM includes several process temperatures and uses the microprocessor to calculate the velocity based on the built-in process temperature measurement.

**GAS CALIBRATION**

The customer has a choice of a laboratory calibration or a gas correlation calibration. Air calibrations are performed in the Kurz Model 400D NIST traceable wind tunnel.

**SENSOR PROTECTION**

The 454FTB circuitry includes circuitry to prevent an over-temperature condition caused by a sensor, wiring or component failure. Our sensors will not overheat at zero flow, unlike most competitive devices because of our constant temperature sensor control method and the power limiting design.

**AIR PURGE SENSOR CLEANING SYSTEM**

The Model 454PFTB has a special nozzle in the sensor window for use with the Model 146 Air Sensor Cleaning System. The sensor cleaning is accomplished by a short, high pressure blast of air (sonic velocity) directed at the velocity and temperature sensors. Kurz provides solenoid valves and air blow-down tanks to allow periodic or on-demand cleaning. The 454PFTB has a built-in timer and relay to initiate the purge cycle. The measurement value is "held" during the purge cycle. The air blow-down tank uses customer supplied compressed air (instrument quality) at 60 to 125 PSIG. The average cleaning air consumption is less than 0.125 SCFM. The Model 454PFTB is designed to measure air flow only at ambient pressure. Canadian Registration (CRN) is not available for the Model 454PFTB. The primary application is for extremely dirty stacks and ducts having dry particulate matter that may build up on the sensor. Applications include fossil-fueled power boilers, municipal waste incinerators and combustion air flow situations in which fly ash is entrained.

**SENSOR ELECTRONICS**

The Series 454FTB has several innovations which improve performance, reduce cost, and provide extraordinary flexibility. The patented digital sensor control circuit (US Patent 7,418,878) uses an efficient switching power supply. The single PCB has an EEPROM loaded with the PCB serial number, calibration coefficients, and component values that ensures the safety of the data. The sensor electronics includes a sensor lead resistance compensation circuit, which is extremely important for long sensor wires, rapid gas temperature changes, and large temperature gradients between the sensor and the ambient air.



**SPECIFICATIONS** *cont'd.*

**Meter Filter Time Constant:**

Selectable 0 to 600 seconds

**Safety Approvals:**

CSA Non-Incendive Approval:  
IEC 79-15 and EN60079-0/15

ATEX Non-Incendive Approval:  
EN60079-0/15 and EN61241-1

CSA Explosion-Proof Approval:  
IEC 79-01 and EN60079-01

ATEX Flame-Proof Safety Approval:  
EN 60079-0/1

**Note:** See Kurz product manual for complete Safety Approvals Specifications.

**CE Directives:**

EMC, ATEX, LVD and PED.  
Consult Kurz for details

**Serial Port Baud Rate:**

User selectable: 9600, 14,400,  
19,200, 38,400, 57,600

**Communication Ports:**

RS485 Modbus ASCII or  
RTU Mode, and USB

**Digital Inputs:**

Two, contact closure, TTL

**Analog Input:**

One, 4-20mA, non-isolated

**LCD:** Back-lit two-line alphanumeric  
with 16 characters per line

**LCD Update:** Every two seconds

**Keypad:** 20-button membrane  
mounted inside enclosure

**Display/Keypad Orientation:**

Adjustable in 90° increments  
to accommodate viewing  
orientation

**Electronics Enclosure**

**Orientation:** 0° or 180° for viewing  
(Feature 1)

**Memory:** EEPROM for all important  
data, with automatic sensor  
identification; Flash EEPROM for  
program memory

**Net Weight/Shipping Weight:**

DC version: 4lbs/5lbs;  
AC version: 6lbs/8lbs,  
add 4lbs/5lbs for remote option

**TECHNICAL DESCRIPTION** *cont'd.*

**FIRMWARE**

The onboard menu system is easy to use and intuitive. The flow meter data (velocity, mass rate, volumetric rate, and temperature) can be displayed in a user-selectable form and viewed through the window in the lid. A local keypad can be accessed to navigate through the onboard menu system to display various flow and diagnostic data as well as enter basic and advanced setup options. A user code is required for programming and entering configuration data or performing test and diagnostic utilities.

**SELF-DIAGNOSTICS**

The 454FTB performs an extensive systems check upon power-up, continuously monitors the sensor inputs/outputs, and verifies the integrity of the sensor wiring and the measurements.

**PROGRAMMABLE CORRECTION FACTORS**

A multi-point Variable Correction Factor can be used to correct the flow calibration data to meet in-situ flow tests over the entire velocity range such as for EPA stack flow monitors. A Sensor Blockage Correction Factor (SBCF) can be used to correct area reduction caused by the sensor support. A single-point correction factor may also be used.

**METER FILTER TIME CONSTANT**

A digital filter time constant can be set for the flow calculation, which affects the displayed values and the 4-20 mA outputs. The time constant can be set from 0 to 600 seconds.

**COMPATIBILITY WITH SERIES 155 MASS FLOW COMPUTERS**

The 454FTB is fully compatible with the inputs and features of the Series 155 Mass Flow computer. DC powered units can be directly powered by the Series 155. This feature is used when two or more Model 504FTBs are used in a multi-point velocity array. Please see the Series 155 brochure.

**SELECTABLE STP CONDITIONS**

The mass flow calibration data is referenced to the Kurz laboratory standard of 77°F/14.69 PSIA (25° C/101.325 kPa). The user may change the STP conditions to suit his requirement without affecting the calibration data.

**4-20 mA OUTPUTS**

The 4-20mA outputs can be wired as optically isolated loop-powered outputs or non-isolated, self powered outputs. The user can easily re-calibrate the 4-20 mA outputs using the Calibrate Analog Output menu in the onboard menu system or through the HART interface.

**NAMUR NE43 COMPLIANCE**

Kurz meets the NAMUR NE43 recommendation for the 4-20 mA outputs to indicate a sensor or system fault. An NE43 alarm can be selected as high or low. This feature frees up the alarm/relays so that the user can set-up the relays for other needs.

**BUILT-IN "ZERO-MID-SPAN" DRIFT CHECK/CALIBRATOR**

The B-Series Flow Transmitters have a Drift Check feature that meets the U.S. EPA requirements for CEM Stack Flow Monitors. The B-Series have a built-in independent voltage source that is used to drive the 4-20mA output for the Drift Check tests. A Drift Check setup menu is available to configure the signal level and duration for the Drift Checks at Zero, Mid, and Span. Drift Checks can be initiated with a contact closure, through a MODBUS command, using an automatic internal timer, through the HART interface, or using the local onboard menu system.

**GREENHOUSE GAS REPORTING**

The EPA requires certain facilities to report GHG emissions. This rule is contained in US Code of Federal Regulations Title 40, Part 98. Kurz thermal mass flow meters meet the certification requirement in 40 CFR 98.34(c)(1) required by the Mandatory GHG Reporting regulation and are approved for this application.

**RELAYS - ALARMS/PULSED TOTALIZER OUTPUT/PURGE OUTPUT**

The 454FTB can be ordered with two solid-state optically isolated relays. The relay outputs can be user configured for alarm outputs, pulsed totalizer output, or air purge cleaning. If no relays are ordered, the alarm functions are available. Totalizers can be automatically reset at a specific total quantity (10,000 SCF).



# SERIES 454FTB SINGLE-POINT INSERTION THERMAL MASS FLOW TRANSMITTERS

## TECHNICAL DESCRIPTION cont'd.

### ANALOG INPUT

One non-isolated 4-20mA input for use as a remote set-point for the built-in PID Flow Controller.

### PID FLOW CONTROLLER

The 454FTB includes the capability of controlling the velocity or flow rate through the use of the user's control valve, damper or position commanded 4-20 mA interface device. The set-point can be internal or remote.

### USB PORT

A USB port for terminal operations includes a COM emulator driver that can be accessed using a terminal emulator program to remotely echo the display and keypad functions and upload/download the system configuration and calibration data files using XMODEM protocol. Process data can be initiated manually through the Log Mode menu from the remote terminal/keyboard or the local display/keypad. The information can also be obtained automatically by configuring the Serial Data Logging through the onboard menu system.

### HART

The Series 454FTB can be ordered with the HART communication interface. The HART protocol is a recognized and accepted standard in the process control industry. This interface provides the benefits of remote configuration, remote diagnostic monitoring, and the ability to do testing online using available handheld configurators.

### MODBUS

The Modbus local network protocol (ASCII or RTU) is included. Modbus is extremely useful for accessing most features, including configuration upload and download.

## ORDERING INFORMATION

### FLOW TRANSMITTER SELECTION

Table 1 lists the Series 454FTB Model number, Parent Number and Major Features. Table 2 lists the Baseline ( $V^*$ ) Full Scale Velocity for each Gas Type. Table 3 lists the Flow Factor ( $F^*$ ) Equation for each Gas Type. See definitions on page 11.

TABLE 1: SERIES 454FTB SELECTION TABLE

Model Number	Parent Number	Sensor Support Dia.	Process Temp. Rating	Air Purge	Safety Approvals
454FTB-08-HT	756051	1/8"	HT	No	NI, XP/FP
454FTB-08-HHT	756052	1/8"	HHT	No	NI, XP/FP
454FTB-12-HT	756053	3/4"	HT	No	NI, XP/FP
454FTB-12-HHT	756054	3/4"	HHT	No	NI, XP/FP
454FTB-16-HT	756055	1"	HT	No	NI, XP/FP
454FTB-16-HHT	756056	1"	HHT	No	NI, XP/FP

TABLE 2: BASELINE  $V^*$  VELOCITY RANGES (See Notes 1, 2, 3)

Model Number	VELOCITY SFPM (NMPS)					
	Gas Category and Gas Type					
	1 Air, N <sub>2</sub> , O <sub>2</sub> , Ar, CO <sub>2</sub> , Dry Cl <sub>2</sub>	2 Methane, Digester Gas, Dry Ammonia	3 Ethylene	4 Ethane	5 Helium, Propane, Butane	6 Hydrogen
454FTB-08-HT 454FTB-12-HT 454FTB-16-HT to 125°C	18,000 (84)	17,000 (79)	15,000 (70)	13,300 (62)	10,000 (47)	6,000 (28)
454FTB-08-HT 454FTB-12-HT 454FTB-16-HT 454PFTB-16-HT to 260°C	18,000 (84)	N/A	N/A	N/A	N/A	N/A
454FTB-08-HHT 454FTB-12-HHT 454FTB-16-HHT to 500°C	18,000 (84)	N/A	N/A	N/A	N/A	N/A

Note 1: See nomenclature for the complete definition of gas group number and gas type.

Note 2: SFPM: Standard feet-per-minute (Ref.: 77°F, 14.69 PSIA).

NMPS: Normal meters-per-second (Ref.: 0°C, 760 mm Hg).

NMPS = 0.00466 x SFPM (approximate).

Note 3: The baseline ( $V^*$ ) VELOCITY for each mass flow transmitter model number and for each type of gas is the maximum velocity at standard conditions (see Note 2).

TABLE 3: FLOW FACTOR ( $F^*$ ) EQUATIONS

Gas	DR <sub>p</sub>	Equations
Category 1: Air, N <sub>2</sub> , Ar, CO <sub>2</sub> , O <sub>2</sub> , Dry Cl <sub>2</sub>	Less than 1.333	$F^* = DR_p$
	Greater than 1.333	$F^* = 1.333$
Category 2: Methane, Digester Gas, Dry Ammonia	Less than 0.945	$F^* = 1.059DR_p$
	Greater than 0.945	$F^* = 1.000$
Category 3: Ethylene	Less than 0.833	$F^* = 1.2DR_p$
	Greater than 0.833	$F^* = 1.0$
Category 4: Ethane	Less than 0.739	$F^* = 1.353DR_p$
	Greater than 0.739	$F^* = 1.000$
Category 5: Helium, Propane, Butane	Less than 0.555	$F^* = 1.8DR_p$
	Greater than 0.555	$F^* = 1.00$
Category 6: Hydrogen	Less than 0.333	$F^* = 3.0DR_p$
	Greater than 0.333	$F^* = 1.000$

# SERIES 454FTB SINGLE-POINT INSERTION THERMAL MASS FLOW TRANSMITTERS

## NOMENCLATURE:

PROCESS TEMPERATURE RATING		
Identifier	Description	Range
HT	High Temperature	-40°F to 500°F (-40°C to 260°C)
HHT	Very High Temperature	-40°F to 932°F (-40°C to 500°C)

SENSOR TYPE	
Identifier	Description
FD2	Fast Dual Metal-Clad™ Velocity and Temperature Sensor; all-welded construction. 0.105" diameter sensor stings

SAFETY APPROVALS	
Identifier	Description
NI	Non-Incendive, CSA and ATEX
XP/FP	Explosion-Proof/Flame-Proof, CSA and ATEX

GAS CATEGORY AND GAS TYPE	
Category	Gas Type
1	Air, Nitrogen, Oxygen, Argon, Carbon Dioxide, Dry Chlorine
2	Methane, Digester Gas, Dry Ammonia
3	Ethylene
4	Ethane
5	Helium, Propane, Butane
6	Hydrogen

### Part Number Generation Procedure

With the selected Parent Number, specify the entire Part Number by selecting an Option for each Feature as shown in the example below. Feature Options in Bold type indicate the most available models, other options usually require a longer delivery time.

Example Part Number for a Model 454FTB-16-HHT:

756056	D	32	F	4	F	077	M	01	A	015	B	1392
Parent Number	F1	F2	F3	F4	F5	F6	F7	F8	F9	F10	F11	F12

FEATURE 1: ELECTRONICS ENCLOSURE CONFIGURATION AND INPUT POWER (See Note 1)	
Option	Description
A	Directly Attached Electronics Dual-Chamber Enclosure, AC power, LCD/Keypad.
B	Directly Attached Electronics Dual-Chamber Enclosure, AC power, without LCD/Keypad.
C	Directly Attached Electronics Dual-Chamber Enclosure rotated 180° for viewing, AC power, LCD/Keypad.
D	Remote Electronics Dual-Chamber Enclosure, AC power, LCD/Keypad.
E	Remote Electronics Dual-Chamber Enclosure, AC power, without LCD/Keypad.
F	Directly Attached Electronics Dual-Chamber Enclosure, 24V DC power, LCD/Keypad.
G	Directly Attached Electronics Dual-Chamber Enclosure rotated 180° for viewing, 24V DC power, LCD/Keypad.
H	Directly Attached Electronics Single-Chamber Enclosure, 24V DC power, without LCD/Keypad.
I	Remote Electronics Dual-Chamber Enclosure, 24V DC power, LCD/Keypad.
J	Remote Electronics Single-Chamber Enclosure, 24V DC power, without LCD/Keypad.

**Note 1:** The conduit or cable seal must be installed by an experienced and careful installer to prevent water intrusion into the enclosure and to maintain the enclosure rating. Failure to properly install the conduit seals may void the Kurz warranty and may compromise the safety approval rating.

**Note 2:** Stainless Steel Identification Tags are available. Customer must provide labeling information up to four lines of text with 32 characters each line.

SUMMARY OF FEATURES	
Feature	Feature Description
1	Electronics Enclosure Configuration and Input Power, LCD/Keypad
2	Sensor Material/Sensor Support and Flange Material
3	Sensor Support Length
4	Process Temperature Compensation
5	Optional Flange Connection Size and Rating
6	Optional Flange U Dimension
7	Gas Velocity Calibration Data Range
8	Specialty Gas Velocity Calibration
9	Safety Approvals
10	Process Pressure
11	Analog & Digital Inputs/Outputs
12	Process Temperature



# SERIES 454FTB SINGLE-POINT INSERTION THERMAL MASS FLOW TRANSMITTERS

FIRST DIGIT OF FEATURE 2: SENSOR MATERIAL	
Option	Description
3	Alloy C-276
7	Alloy C-276 with Abrasion-Resistant Chromium Nitride Coating (CrN)

SECOND DIGIT OF FEATURE 2: SENSOR SUPPORT AND FLANGE MATERIAL (Note 1)	
Option	Description
2	316L Stainless Steel
3	Alloy C-276
8	Alloy C-276 with PTFE Compound Coating cured for chemical resistance. Includes support, sensor and flange: FD2 sensors only, temperature rating of 260°C Max.

Note 1: Sensor Support Material and Optional Flange Material must be the same, see Feature 5.

FEATURE 3: SENSOR SUPPORT LENGTH L			
Option	Support Length L	Option	Support Length L
B	6" (125°C Max)	J	30"
C	9" (260°C Max)	K	36"
D	12"	M	48"
F	18"	P	60"
H	24"		

FEATURE 4: PROCESS TEMPERATURE COMPENSATION	
<p>The influence of temperature on the thermal properties of gases requires temperature compensation of the Thermal Mass Flow Sensor for repeatability and accurate measurements. Standard Temperature Compensation (STC) is used for applications in which the process temperature is below 125°C over a moderate velocity range (Option 1); or below 260°C over more limited velocity range (Option 2).</p> <p>If the process temperature and gas velocity vary widely, Velocity Temperature Mapping (VTM) is recommended. VTM (Options 3, 4) includes several calibrations. The multiple velocity calibrations are entered into the Microprocessor which performs a double interpolation between the velocity calibration curves using the built-in process gas temperature measurement. The temperature compensation is based upon air, therefore, the accuracy at a high temperature when using gases other than Air, Nitrogen or Oxygen may be reduced unless a gas correlation is specified (see feature 8).</p>	
Option	Description
1	Standard Temperature Compensation (STC) over process temperature range from -40°C to +125°C. Accuracy: $\pm$ (1% Reading + 20 SFPM) above or below 25°C (see note 1).
2	Standard Temperature Compensation (STC) over process temperature range from 0°C to 260°C. Accuracy: $\pm$ (2% Reading + 20 SFPM) above or below 125°C (see note 1).
3	Velocity-Temperature Mapping (VTM) with data sets over process temperature range from 0°C to 260°C. Accuracy: $\pm$ (2% reading + 20 SFPM).
4	Velocity-Temperature Mapping (VTM) with data sets over the process temperature range from 0°C to 500°C. Accuracy: $\pm$ (3% reading + 30 SFPM), specify process temperature range. HHT Models.

Note 1: An accuracy specification of  $\pm$  (0.025%/°C Reading + 0.25 SFPM/°C) should added for temperatures above or below standard.

## FEATURE 5: OPTIONAL FLANGE CONNECTION SIZE AND RATING

### How to determine the U, L, and L2 dimensions for a flange connection

When ordering a flange, you must specify the U dimension, and verify that the sensor support length L and L2 are appropriate for the Process Temperature. Kurz recommends that the centerline of the sensor be located at the center of the pipe or duct, and that experimental flow profile tests be made to obtain the velocity profile correction factor (VCF) and enter it into the 454FTB. Refer to the outline drawings in the Series 454FTB Brochure. **Note:** Flange material must match Sensor Support Material (Feature 2).

U = The dimension between the centerline of the mass flow sensor and the flange mounting surface. The minimum U dimension is 4.0".

L = The length of the sensor support tube (Feature 3).

L2 = The length of sensor support between the flange mounting surface and the sensor support fitting. The minimum L2 is 5" for HT process temperatures and 8" for HHT process temperatures.

L = U + L2 - 2.00"

Option	Sensor Support Diameter	Description
A	1/2", 3/4", 1"	No flange connection
B	1/2"	1/2", Class 150, ANSI B16.5
C	1/2"	1/2", Class 300, ANSI B16.5
D	1/2", 3/4"	3/4", Class 150, ANSI B16.5
E	1/2", 3/4"	3/4", Class 300, ANSI B16.5
F	1/2", 3/4", 1"	1", Class 150, ANSI B16.5
G	3/4", 1"	1", Class 300, ANSI B16.5
H	3/4", 1"	1 1/4", Class 150, ANSI B16.5
I	3/4", 1"	1 1/4", Class 300, ANSI B16.5
J	3/4", 1"	1 1/2", Class 150, ANSI B16.5
K	3/4", 1"	1 1/2", Class 300, ANSI B16.5
L	3/4", 1"	2", Class 150, ANSI B16.5
M	3/4", 1"	2", Class 300, ANSI B16.5
N	1"	2 1/2", Class 150, ANSI B16.5
P	1"	2 1/2", Class 300, ANSI B16.5
S	1"	3", Class 150, ANSI B16.5
T	1"	3", Class 300, ANSI B16.5
U	1"	4", Class 150, ANSI B16.5
V	1"	4", Class 300, ANSI B16.5

Note: Flange material must match the Sensor Support Material (Feature 2).

FEATURE 6: OPTIONAL FLANGE U DIMENSION	
Directions	
<p>Divide the U Dimension (inches) by 100, round off the resulting number to the right of the decimal point to three significant digits, enter the resulting three digit number without the decimal point. Enter 000 for no flange connection. <math>U_{min} = 4"</math></p> <p>Example: The U Dimension is 7.74"; Enter 077.</p>	



# SERIES 454FTB SINGLE-POINT INSERTION THERMAL MASS FLOW TRANSMITTERS

FEATURE 7: GAS VELOCITY CALIBRATION DATA RANGE SFPM (NMPS) (Note 1)			
Option	Velocity	Option	Velocity
A	$V_{MAX}$	M	6,000 (28.0)
B	300 (1.4)	P	9,000 (41.9)
C	600 (2.8)	R	12,000 (56)
E	1,000 (4.7)	T	15,000 (70)
G	2,000 (9.3)	V	18,000 (84)
I	3,000 (14)	X	24,000 (112)
K	4,000 (18.6)		

**Note 1:** The Gas Velocity ( $V_g$ ) must be equal to or less than  $V_{MAX}$  for the Process Absolute Temperature and Pressure and for the specific Gas Category and Gas Type as determined using Tables 2, 3 and Equations 1, 2.

FEATURE 8: SPECIALTY GAS VELOCITY CALIBRATION	
There are two Specialty Gas Velocity Calibration methods available:	
1. Laboratory Gas Velocity Calibration.	
2. Correlation Gas Velocity Calibration in which the Insertion Mass Flow Transmitter is calibrated in air and experimentally derived correlation factors are used to obtain calibration data for the specialty gas.	

FEATURE 8: SPECIALTY GAS VELOCITY CALIBRATION (Note 1)		
Laboratory Calibration Option	Gas Type Option	Correlation Calibration Option
01	Air	—
07	Compressed Air	—
—	Dry Ammonia	56
08	Argon	58
—	Butane	60
14	Carbon Dioxide	64
—	Dry Chlorine	68
20	Ethane	70
22	Ethylene	72
26	Helium	—
28	Hydrogen	—
32	Methane	82
35	Digester Gas 50% CH <sub>4</sub> , 50% CO <sub>2</sub>	85
36	Digester Gas 60% CH <sub>4</sub> , 40% CO <sub>2</sub>	86
37	Digester Gas 70% CH <sub>4</sub> , 30% CO <sub>2</sub>	87
40	Nitrogen	90
44	Oxygen (Note 2)	94
46	Propane	96

**Note 1:** Laboratory Gas calibrations are performed with gases of high purity and are NIST Traceable. Customer must specify calibration pressure (Feature 10). Propane to 50 PSIA, all other gasses to 150 PSIA. Correlation calibrations are based on experimental data correlated to an air calibration at ambient pressure and temperature. The user's flow element is calibrated in air, and an additional calibration data sheet is made for the specialty gas based upon the correlation factors. Add  $\pm 5\%$  of Reading to the accuracy specifications when using a gas correlation calibration. All correlations include VTM.

**Note 2:** It is the customer's responsibility to insure that the Mass Flow Element is clean of Hydrocarbons and is safe for oxygen use. (Oxygen cleaning is optional.)

FEATURE 9: SAFETY APPROVALS/ENCLOSURE MATERIAL (Note 1)	
Option	Description
A	Non-Incendive (NI), CSA, ATEX, and IECEx Aluminum enclosures Type 4, IP66 Ex nA II Gc, T6, T5, T4 or T130°C (electronics enclosure) Ex nA II Gc, T5 or T3 (sensing element) Applies to Feature 1, options A through J
B	Explosion-Proof/Flame-Proof, CSA, ATEX, and IECEx Aluminum enclosures Type 4, IP66 Ex d IIB + H2 Gb, T6, T4, T110°C or T130°C (electronics enclosure) Ex d IIB + H2 Gb, T4 or T3 (sensing element) Applies to Feature 1, options A through J

**Note 1:** See Specifications, Page 5.

FEATURE 10: PROCESS PRESSURE	
Enter the Absolute Pressure (PSIA), rounded off to 3 digits. Example: For a Process Absolute Pressure of 14.7 PSIA, enter 015; for 150 PSIA, enter 150.	

FEATURE 11: ANALOG AND DIGITAL INPUTS/COMMUNICATIONS							
Option	Analog & Digital Inputs				Communication Protocols		
	No. of Alarm Relay Outputs (DO)	No. of 4-20mA Outputs (AO)	No. of Digital Inputs (DI)	No. of 4-20mA Inputs (AI)	USB	Modbus RS-485 RTU or ASC II	HART (FSK 7.0)
B	0	2	0	0	Yes	Yes	No
C	2	2	2	1	Yes	Yes	No
E	2	1	2	1	Yes	Yes	Yes

**Option B provides:**

- Two 4-20 mA outputs for flow rate and/or temperature, NAMUR NE-43 compliance.
- USB, Modbus, and RS-485 communication protocols.

**Option C provides:**

- Two 4-20 mA outputs for flow rate, temperature, EPA Zero-Mid-Span Drift check<sup>3</sup> or PID Flow Control<sup>1,2</sup>, NAMUR NE-43 compliance.
- Two alarm relays for flow rate, temperature, or pulsed flow totalizer.
- External 4-20 mA input.
- Two DI for EPA Zero-Mid-Span Drift Check or Purge Cycle Cleaning.
- USB, Modbus, and RS-485 communication protocols.

**Option E provides:**

- One 4-20 mA output for flow rate, temperature, EPA Zero-Mid-Span Drift check<sup>3</sup> or PID Flow Control<sup>1,2</sup>, NAMUR NE-43 compliance.
- Two alarm relays for flow rate, temperature, or pulsed flow totalizer.
- External 4-20 mA input.
- Two DI for EPA Zero-Mid-Span Drift Check or Purge Cycle Cleaning.
- HART Communication Interface, USB, Modbus, and RS-485 communication protocols.



**Notes:**



- The PID Flow Controller uses one 4-20 mA output for the flow controller.
- The External Input PID Controller requires a 4-20 mA flow reference input.
- EPA Zero-Mid-Span Drift check normally requires a contact closure to verify that the Drift Check has been truly indicated. The contact closure is generated by the Continuous Emissions Monitor Computer at a specific time every day to indicate the Daily Drift Check. Both 4-20mA outputs are used during the Drift Check Calibration procedure.

FEATURE 12: PROCESS TEMPERATURE	
Enter the Absolute Process Temperature ( $^{\circ}\text{Rankin} = ^{\circ}\text{F} + 460$ ) rounded off to 4 digits. Example: For a Process Temperature of 77°F, enter 0537; for 932°F, enter 1392.	



## SERIES 454FTB OUTLINE DRAWINGS

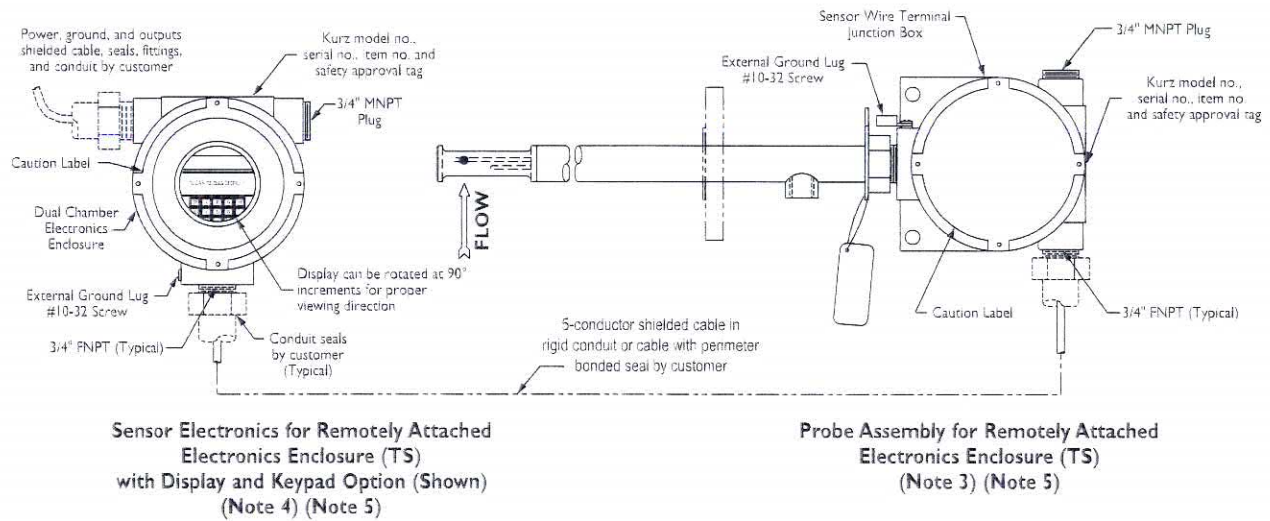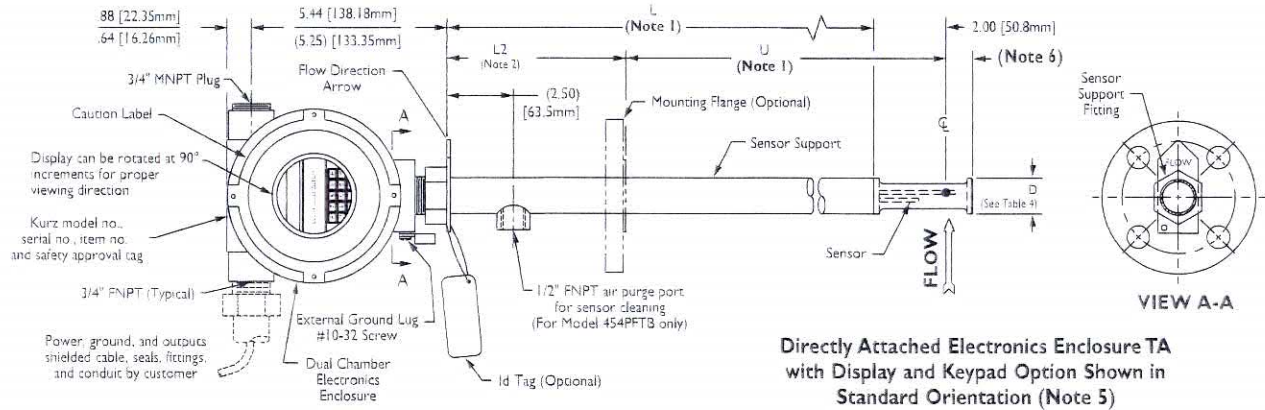

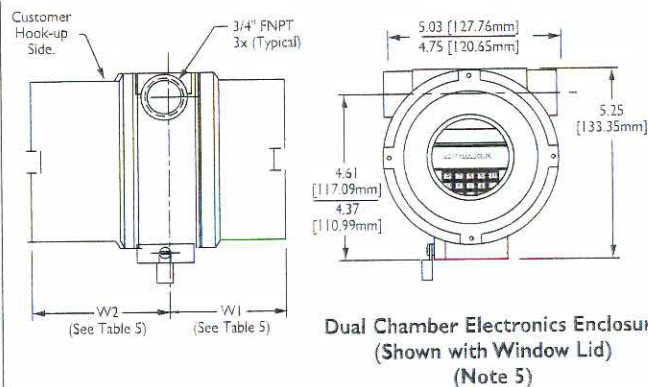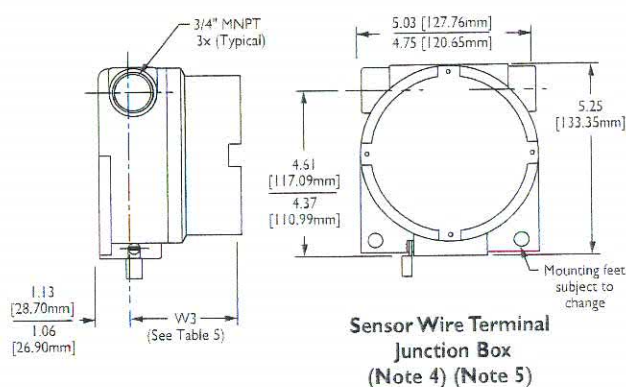

**Notes:**

- 1) For flanged option:  $L = (U + L2 - 2.00 [50.8\text{mm}])$ ,  $U (\text{Min.}) = 4.00 [101.6\text{mm}]$
- 2)  $L2 (\text{Min.})$  for HT to be 5.00 [127mm]  
 $L2 (\text{Min.})$  for -HHT to be 8.00 [203.2mm]
- 3) This probe configuration also used for directly attached, DC powered, with no display.
- 4) Sensor wire terminal junction box used for sensor electronics for DC powered, with no display.
- 5) Enclosure styles and dimensions are subject to change.
- 6) Dimensions for 454FTB-08 (.50 [12.7mm] diameter) to be 0.78 [19.81mm]  
Dimensions for 454FTB-12 (0.75 [19.5mm] diameter) to be 0.78 [19.81mm]  
Dimensions for 454FTB-16 (1.00 [25.4mm] diameter) to be 0.78 [19.81mm]  
Dimensions for 454PFTB-16 (1.00 [25.4mm] diameter) to be 1.35 [34.29mm]
- 7) This configurations allows for probe assembly to be mounted in ZONE 1 area and for remote electronics to be mounted in ZONE 2 area.

**TABLE 4: PROBE DIAMETER DIMENSION**

Model No	D
-08	0.50 [12.7mm]
-12	0.75 [19.5mm]
-16	1.00 [25.4mm]

**TABLE 5: ENCLOSURE DIMENSION (Note 5)**

Input Power	Display/ Keypad	W1 <div>Max Min</div>	W2 <div>Max Min</div>	W3 <div>Max Min</div>
AC	Yes	<div>3.63 [92.20mm] 3.41 [86.61mm]</div>	<div>5.01 [127.25mm] 4.69 [119.13mm]</div>	N/A
AC	No	<div>3.16 [80.26mm] 2.81 [71.37mm]</div>	<div>5.01 [127.25mm] 4.69 [119.13mm]</div>	N/A
24VDC	Yes	<div>3.63 [92.20mm] 3.41 [86.61mm]</div>	<div>5.01 [127.25mm] 4.69 [119.13mm]</div>	N/A
24VDC	No (Note 4)	N/A	N/A	<div>5.01 [127.25mm] 4.88 [123.95mm]</div>
Sensor Wire Terminal J-Box (for remote opt.)		N/A	N/A	<div>3.16 [80.26mm] 2.81 [71.37mm]</div>

**DEFINITIONS FOR THE USE OF TABLES 1, 2, 3**

Equation 1:  $DR_p = \frac{P_p}{P_s} \times \frac{T_s}{T_p}$

Equation 2:  $V_{MAX} = F^* \times V^*$

$V^*$  = Baseline Velocity as listed in Table 2 (SFPM for English units or NMPS for Metric units at standard conditions).

$V_p$  = Process Velocity (SFPM for English units, NMPS for Metric units).

$V_{MAX}$  = Maximum Velocity for a specific Gas Type under process conditions.

$F^*$  = Flow Factor (see table 3).

$T_s$  = Standard Absolute Temperature: 537°R (77°F + 460) for English units or 273°K (0°C) for Metric units.

$T_p$  = Process Absolute Temperature: °R (T°F + 460) for English units or °K (T°C + 273°C) for Metric units.

$P_s$  = Standard Absolute Pressure (14.69 PSIA for English units and Hg for 760mm Metric units).

$P_p$  = Process Absolute Pressure (PSIA for English units and mm Hg for Metric units).

$DR_p$  = Process Gas Density Ratio.

Example: Calculate the maximum allowable Gas Velocity ( $V_{MAX}$ ) for compressed air at 100°F and 135 PSIA for the Model 454FTB-12-HT.

a) From **Table 2**,  $V^* = 18,000$  SFPM

b) Calculate  $DR_p$  from Equation 1:

$$DR_p = \frac{P_p}{P_s} \times \frac{T_s}{T_p} = \frac{135}{14.69} \times \frac{537}{560} = 8.81$$

c) Using **Table 3** for Category I, Air:  $F^* = 1.333$  ( $DR_p$  greater than 1.333)

d) Using Equation 2:  $V_{MAX} = F^* \times V^* = 23,944$  SFPM (111.8 NMPS)



**The Leader in  
Mass Flow Technology for**

**Process and Environmental Measurements**



**Kurz Instruments, Inc.**

**2411 Garden Road, Monterey, CA 93940**

**800-424-7356 ■ 831-646-5911 ■ Fax 831-646-8901**

**[www.kurzinstruments.com](http://www.kurzinstruments.com)**

**e-mail: [sales@kurzinstruments.com](mailto:sales@kurzinstruments.com)**

**IMPORTANT NOTICE:** Specifications are subject to change without notice.

© 2013 Kurz Instruments, Inc. DCN 367521 REV. J-6

**Kurz Instruments, Inc. ■ 2411 Garden Road, Monterey, CA 93940 ■ Tel 800-424-7356  
Fax 831-646-8901 ■ [www.kurzinstruments.com](http://www.kurzinstruments.com) ■ e-mail: [sales@kurzinstruments.com](mailto:sales@kurzinstruments.com)**